


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022897.D
Acq On : 19 Oct 2021 03:53
Operator : SY/MD
Sample : M4137-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGD0

Manual Integrations
APPROVED

MMDadoda
10/19/2021 3:48:23 PM

Quant Time: Oct 19 05:21:26 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 19 04:07:06 2021
Response via : Initial Calibration

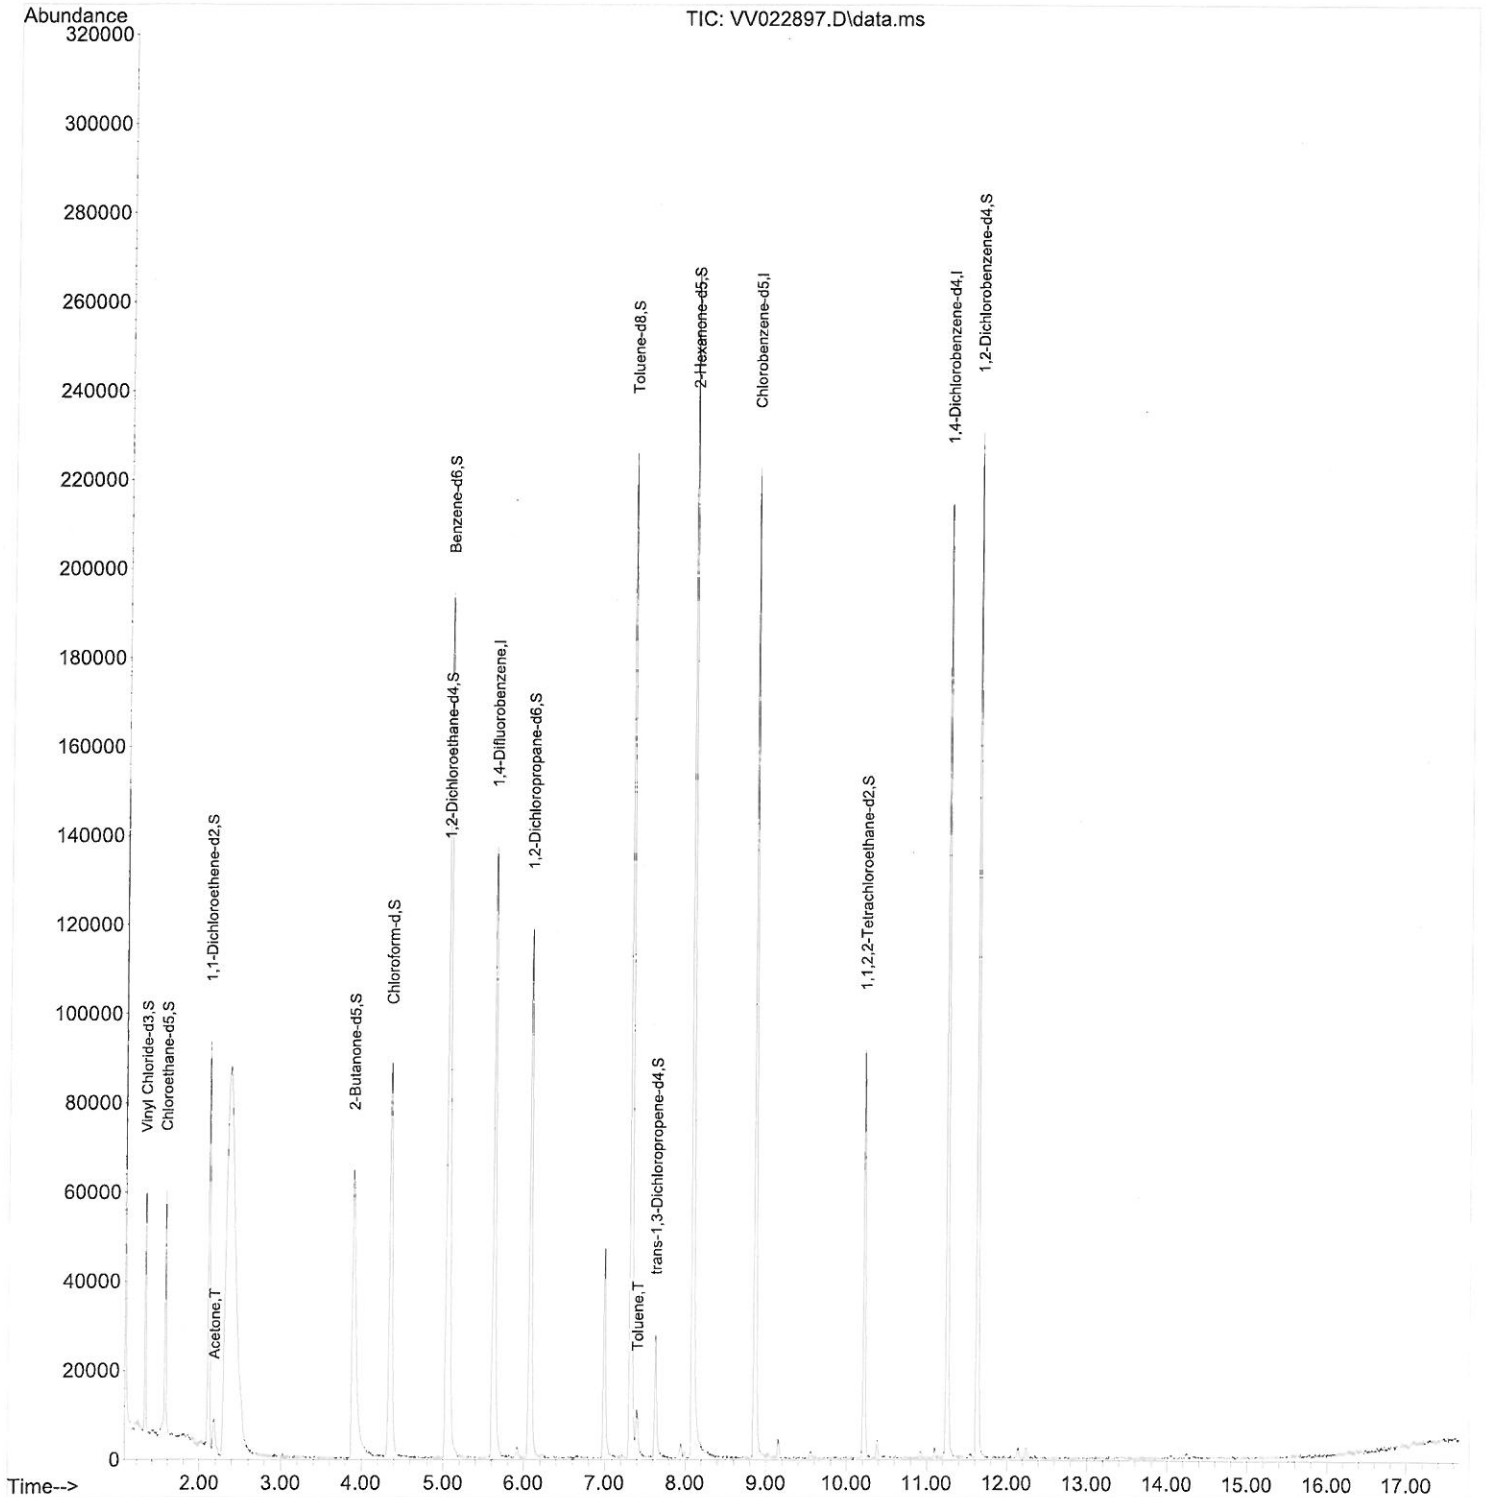

Quantitation Report (Qedit)



Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022897.D
Acq On : 19 Oct 2021 03:53
Operator : SY/MD
Sample : M4137-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGD0

Manual Integrations
APPROVED

MMDadoda
10/19/2021 3:48:23 PM

Quant Time: Oct 19 05:21:26 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 19 04:07:06 2021
Response via : Initial Calibration

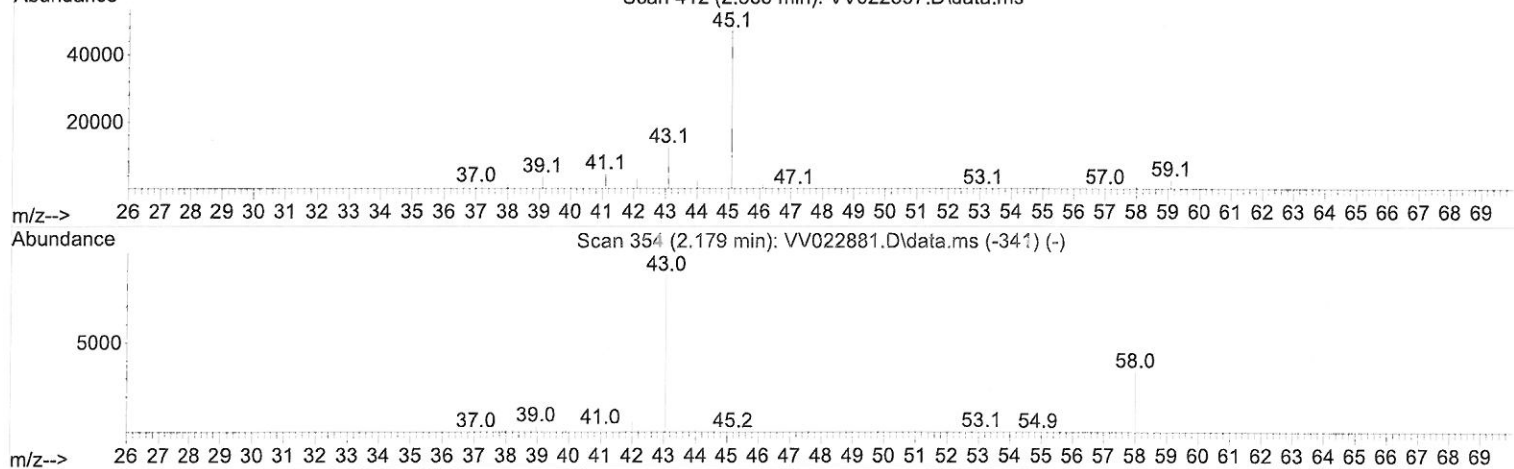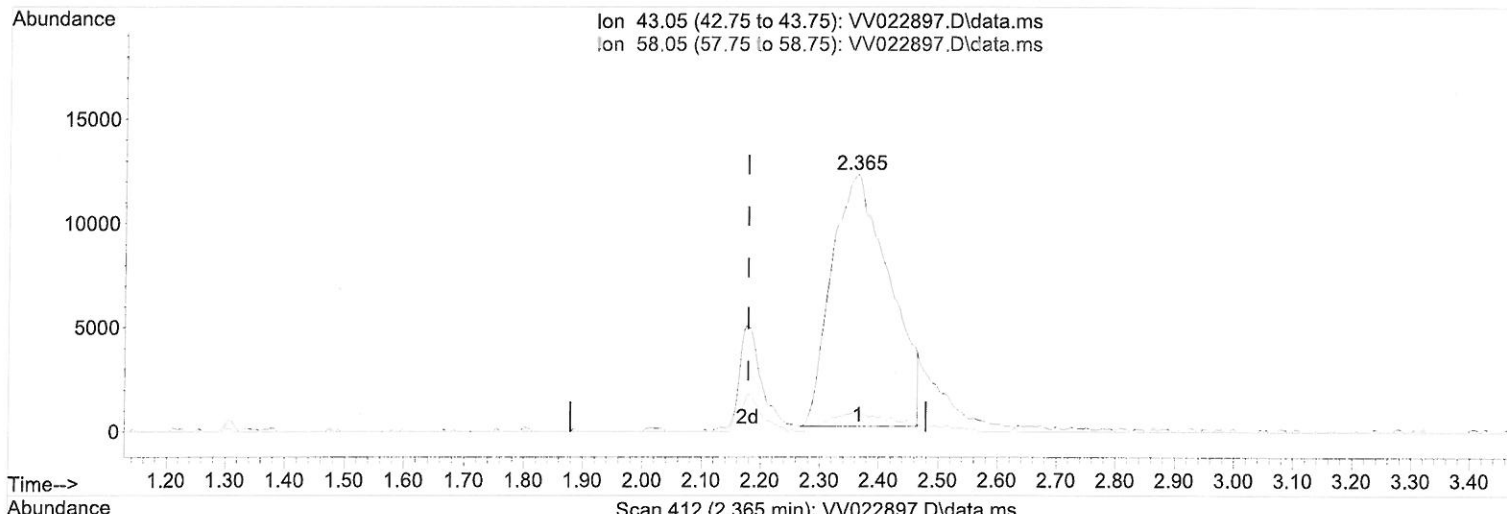

Abundance

Scan 354 (2.179 min): VV022881.D\data.ms (-341) (-)

m/z--> 26 27 28 29 30 31 32 33 34 35 36 37 38 39 40 41 42 43 44 45 46 47 48 49 50 51 52 53 54 55 56 57 58 59 60 61 62 63 64 65 66 67 68 69

TIC: VV022897.D\data.ms

(13) Acetone (T)

2.365min (+ 0.186) 66.78 ug/L

response 81955

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	12.10	0.17
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
 Data File : VV022897.D
 Acq On : 19 Oct 2021 03:53
 Operator : SY/MD
 Sample : M4137-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGD0

Manual Integrations
 APPROVED

MMDadoda
 10/19/2021 3:48:23 PM

Quant Time: Oct 19 05:21:26 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 19 04:07:06 2021
 Response via : Initial Calibration

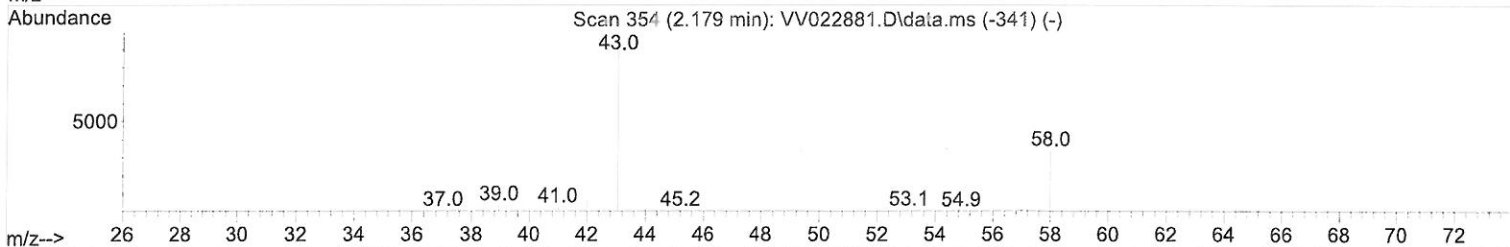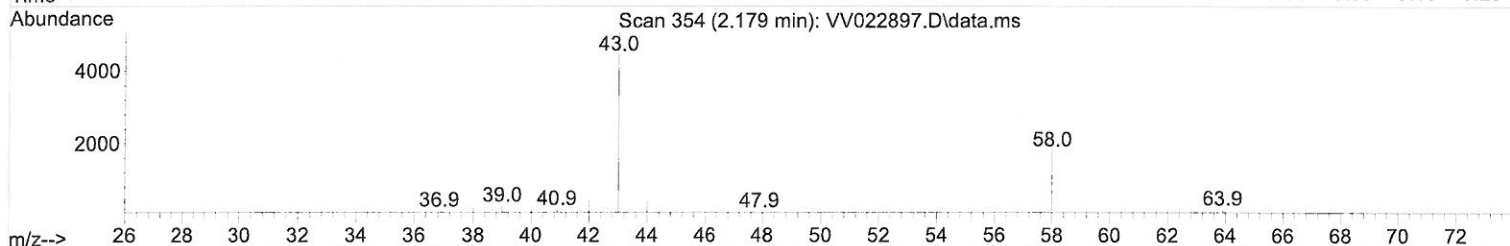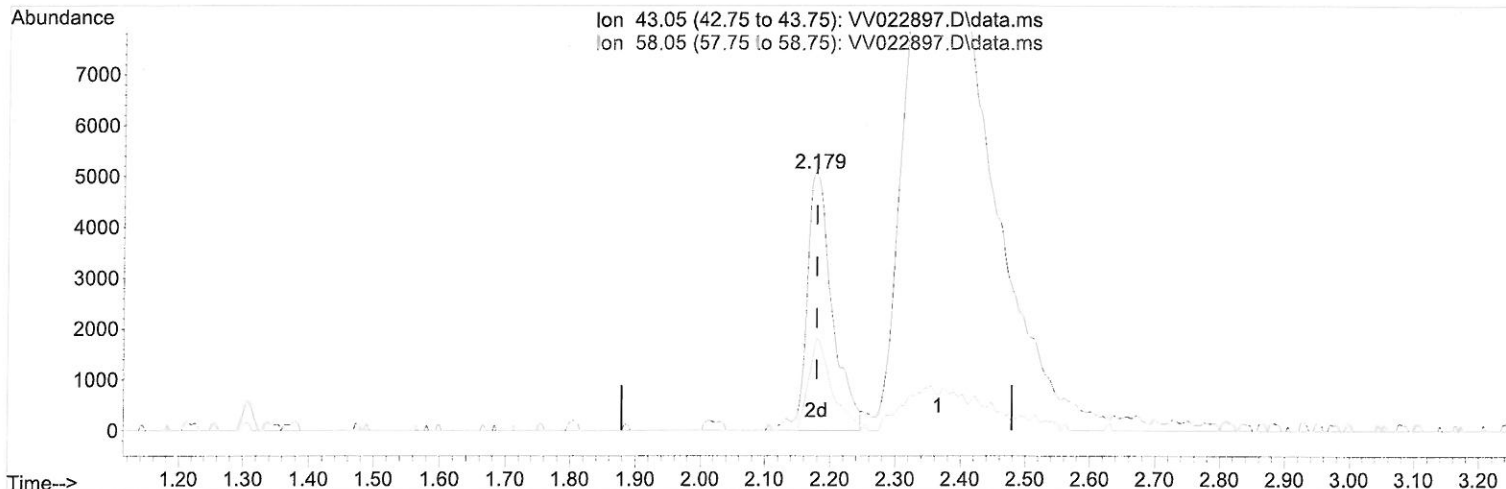

TIC: VV022897.D\data.ms

(13) Acetone (T)

2.179min (-0.000) 11.11 ug/L m

response 13640

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	12.10	1.02
0.00	0.00	0.00
0.00	0.00	0.00

7 MD
 10/27/21

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW101821\
 Data File : VW022897.D
 Acq On : 19 Oct 2021 03:53
 Operator : SY/MD
 Sample : M4137-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGD0

Manual Integrations
 APPROVED

MMDadoda
 10/19/2021 3:48:23 PM

Quant Time: Oct 19 05:21:26 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 19 04:07:06 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	122004	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	126217	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	60675	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	33182	3.953	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	79.000%	
7) Chloroethane-d5	1.568	69	30815	4.085	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	81.800%	
11) 1,1-Dichloroethene-d2	2.108	63	46243	2.808	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	56.200%#	
20) 2-Butanone-d5	3.886	46	115667	52.553	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	105.100%	
24) Chloroform-d	4.349	84	95404	5.515	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	110.400%	
26) 1,2-Dichloroethane-d4	5.034	65	44341	5.281	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	105.600%	
32) Benzene-d6	5.053	84	179556	4.779	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	95.600%	
36) 1,2-Dichloropropane-d6	6.072	67	59293	5.329	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	106.600%	
41) Toluene-d8	7.317	98	150898	4.646	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	93.000%	
43) trans-1,3-Dichloroprop...	7.625	79	17114	4.636	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	92.800%	
46) 2-Hexanone-d5	8.088	63	92884	62.440	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	124.880%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	44707	5.931	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	118.600%	
66) 1,2-Dichlorobenzene-d4	11.625	152	62158	5.525	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	110.600%	
Target Compounds						
13) Acetone	2.179	43	13640m	11.114	ug/L	Qvalue
42) Toluene	7.397	91	7848	0.227	ug/L	98

2 MD
 10/27/21

(#) = qualifier out of range (m) = manual integration (+) = signals summed