

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW101821\
 Data File : VW022859.D
 Acq On : 18 Oct 2021 12:19
 Operator : SY/MD
 Sample : M4207-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Oct 19 01:44:00 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 19 01:43:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	102789	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	121731	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	57541	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	44819	6.34	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	126.80%
7) Chloroethane-d5	1.564	69	36853	5.80	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	116.00%
11) 1,1-Dichloroethene-d2	2.108	63	50001	3.60	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.00%
20) 2-Butanone-d5	3.899	46	45662	24.62	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	49.24%
24) Chloroform-d	4.349	84	71008	4.87	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.40%
26) 1,2-Dichloroethane-d4	5.037	65	33092	4.68	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.60%
32) Benzene-d6	5.053	84	140249	3.87	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	77.40%
36) 1,2-Dichloropropane-d6	6.072	67	41185	3.84	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	76.80%
41) Toluene-d8	7.317	98	126669	4.04	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.80%
43) trans-1,3-Dichloroprop...	7.625	79	14101	3.96	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.20%
46) 2-Hexanone-d5	8.091	63	58201	40.57	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	81.14%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	34447	4.74	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.80%
66) 1,2-Dichlorobenzene-d4	11.625	152	55403	5.19	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.80%
Target Compounds						
16) Methylene chloride	2.510	84	2950	0.35	ug/L	Qvalue 87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022859.D
Acq On : 18 Oct 2021 12:19
Operator : SY/MD
Sample : M4207-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001


Quant Time: Oct 19 01:44:00 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 19 01:43:03 2021
Response via : Initial Calibration

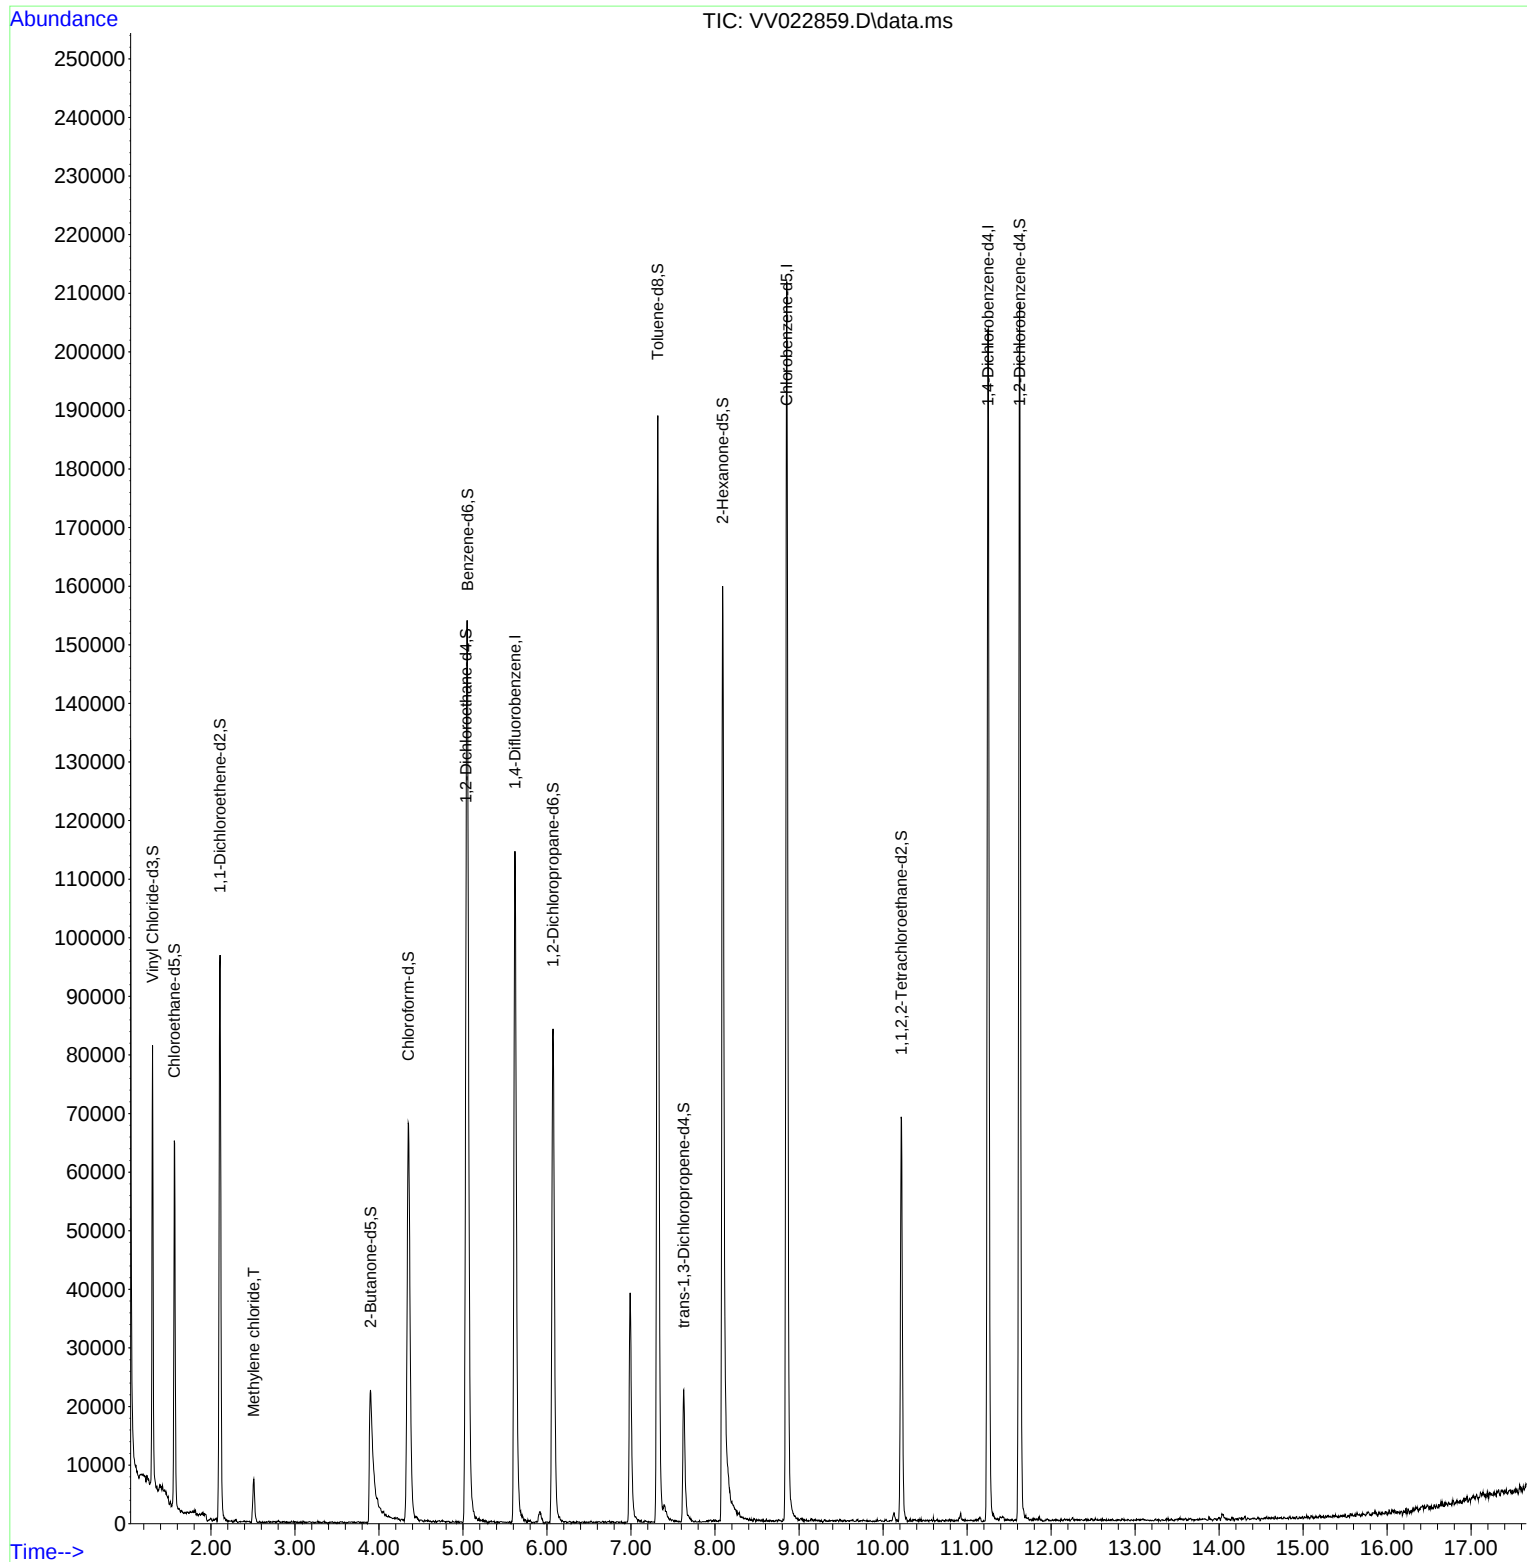

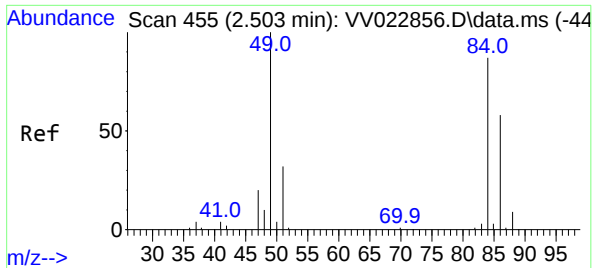

#16
Methylene chloride
Concen: 0.35 ug/L
RT: 2.510 min Scan# 457
Delta R.T. 0.006 min
Lab File: VV022859.D
Acq: 18 Oct 2021 12:19

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

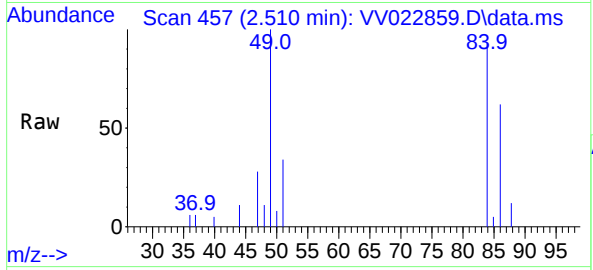

Tgt Ion:	84	Resp:	2950
Ion	Ratio	Lower	Upper
84	100		
86	66.5	45.8	85.2
49	107.0	90.3	167.7

