

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
 Data File : VV022860.D
 Acq On : 18 Oct 2021 12:44
 Operator : SY/MD
 Sample : M4167-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Oct 19 01:44:05 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 19 01:43:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	117079	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	119266	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	56721	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	44242	5.49	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	109.80%
7) Chloroethane-d5	1.564	69	35953	4.97	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.40%
11) 1,1-Dichloroethene-d2	2.105	63	61758	3.91	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	78.20%
20) 2-Butanone-d5	3.905	46	60814	28.79	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	57.58%
24) Chloroform-d	4.349	84	86603	5.22	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.40%
26) 1,2-Dichloroethane-d4	5.037	65	38389	4.76	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.20%
32) Benzene-d6	5.053	84	172555	4.86	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.20%
36) 1,2-Dichloropropane-d6	6.072	67	52767	5.02	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.40%
41) Toluene-d8	7.317	98	144686	4.71	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.20%
43) trans-1,3-Dichloroprop...	7.628	79	16303	4.67	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.40%
46) 2-Hexanone-d5	8.091	63	59387	42.25	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	84.50%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	33528	4.71	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.20%
66) 1,2-Dichlorobenzene-d4	11.625	152	55778	5.30	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.00%
Target Compounds						
16) Methylene chloride	2.507	84	7923	0.81	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022860.D
Acq On : 18 Oct 2021 12:44
Operator : SY/MD
Sample : M4167-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001


Quant Time: Oct 19 01:44:05 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 19 01:43:03 2021
Response via : Initial Calibration

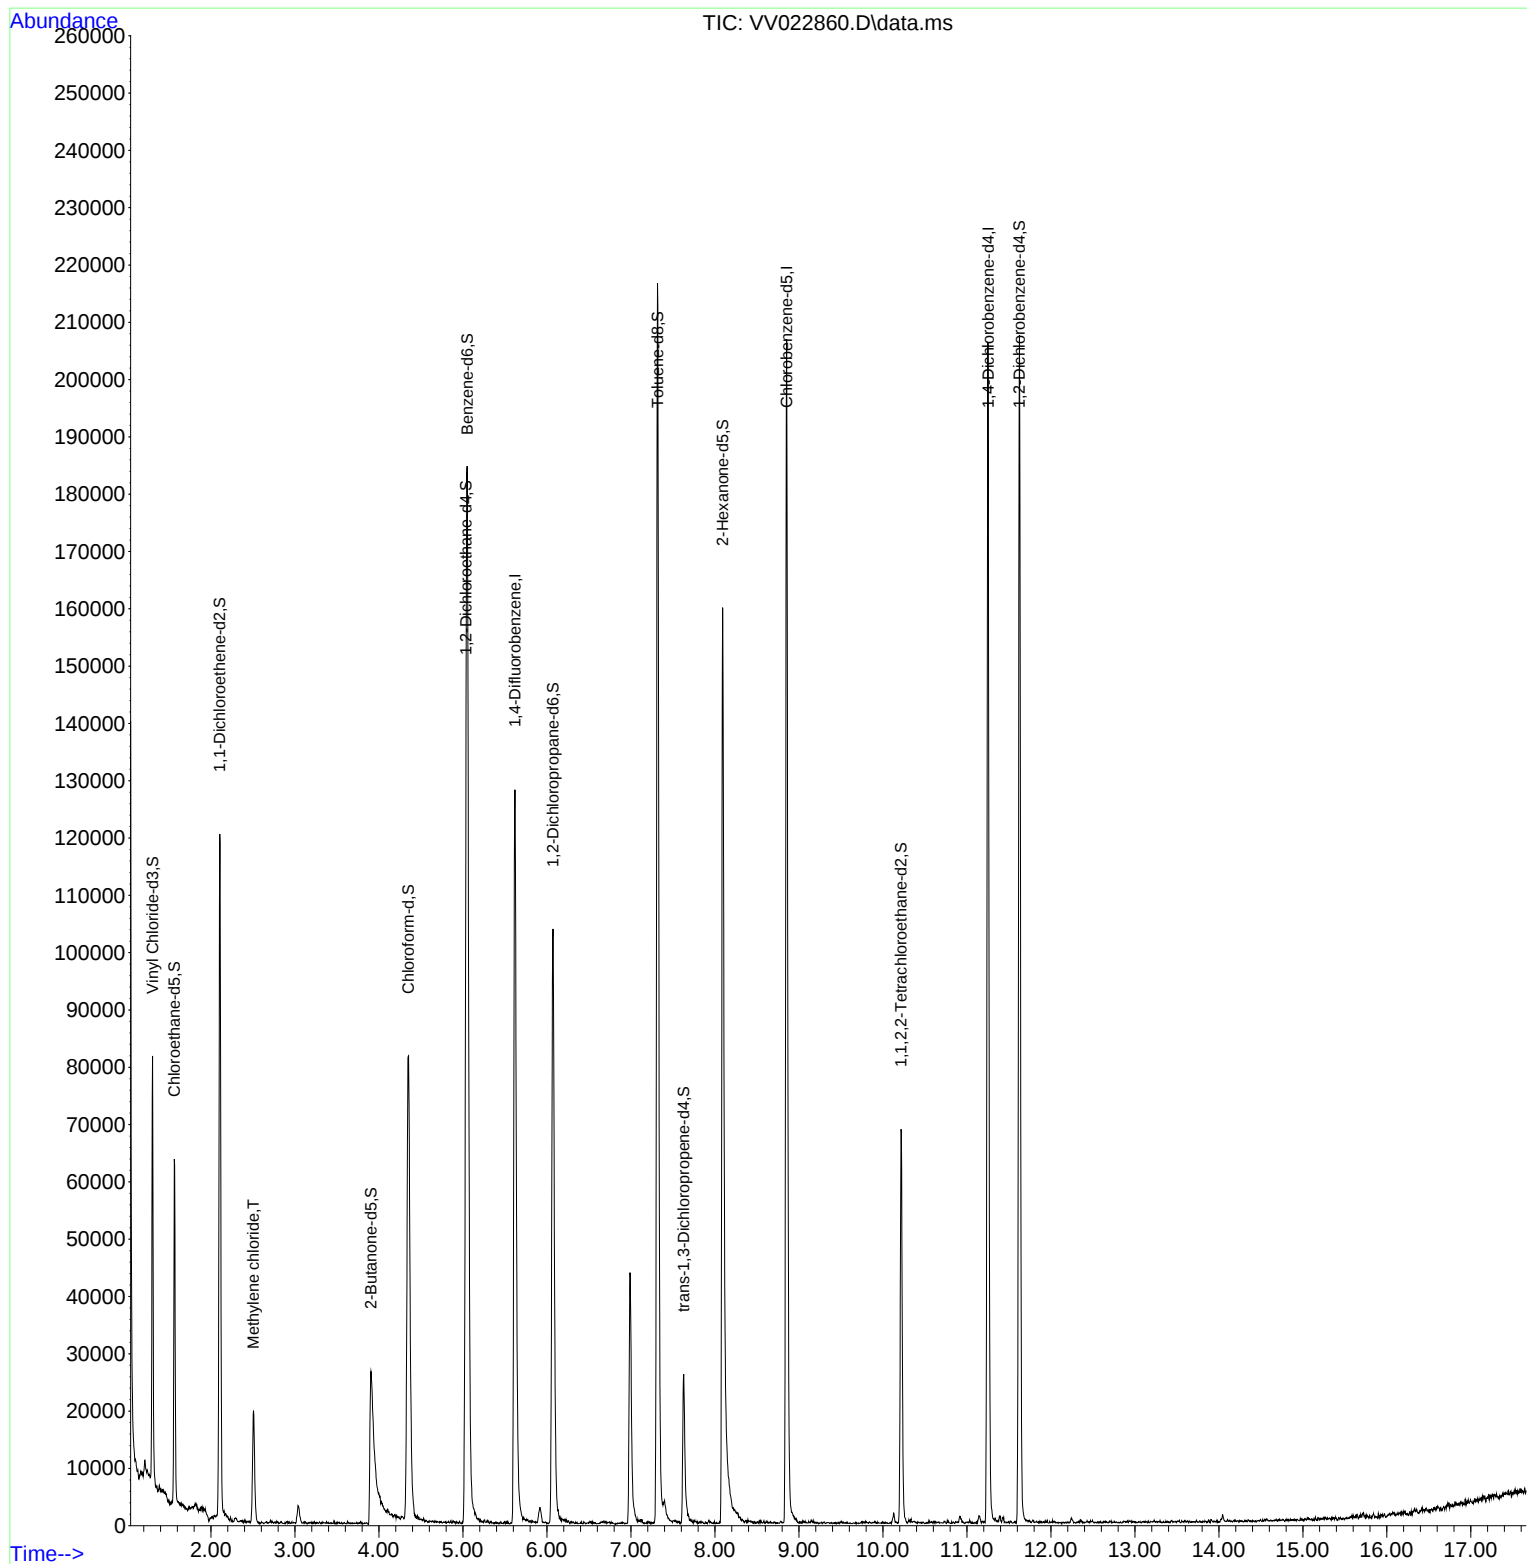

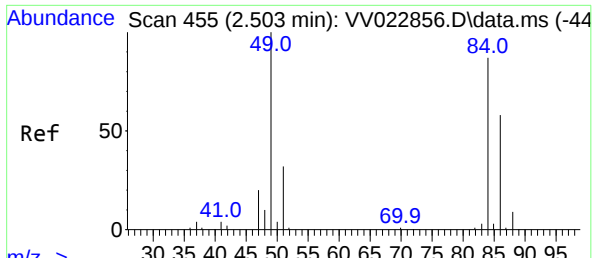

#16
Methylene chloride
Concen: 0.81 ug/L
RT: 2.507 min Scan# 456
Delta R.T. 0.003 min
Lab File: VV022860.D
Acq: 18 Oct 2021 12:44

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

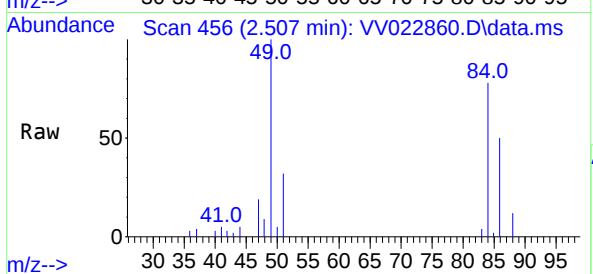

Tgt Ion:	84	Resp:	7923
Ion	Ratio	Lower	Upper
84	100		
86	64.5	45.8	85.2
49	128.7	90.3	167.7

