

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW101821\
 Data File : VW022871.D
 Acq On : 18 Oct 2021 17:04
 Operator : SY/MD
 Sample : M4246-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YAT53

Quant Time: Oct 19 01:45:16 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 19 01:43:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	128911	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	128689	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	60381	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	35187	3.97	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	79.40%
7) Chloroethane-d5	1.568	69	34489	4.33	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	86.60%
11) 1,1-Dichloroethene-d2	2.108	63	54105	3.11	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	62.20%
20) 2-Butanone-d5	3.889	46	95861	41.22	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	82.44%
24) Chloroform-d	4.352	84	92380	5.05	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.00%
26) 1,2-Dichloroethane-d4	5.037	65	42037	4.74	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.80%
32) Benzene-d6	5.053	84	175495	4.58	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.60%
36) 1,2-Dichloropropane-d6	6.072	67	55194	4.86	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.20%
41) Toluene-d8	7.317	98	149232	4.51	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.20%
43) trans-1,3-Dichloroprop...	7.625	79	17130	4.55	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.00%
46) 2-Hexanone-d5	8.088	63	75868	50.02	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.04%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	37563	4.89	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.80%
66) 1,2-Dichlorobenzene-d4	11.625	152	59485	5.31	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.20%
Target Compounds					Qvalue	
13) Acetone	2.175	43	1504	1.16	ug/L	# 44


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022871.D
Acq On : 18 Oct 2021 17:04
Operator : SY/MD
Sample : M4246-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAT53

Quant Time: Oct 19 01:45:16 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 19 01:43:03 2021
Response via : Initial Calibration

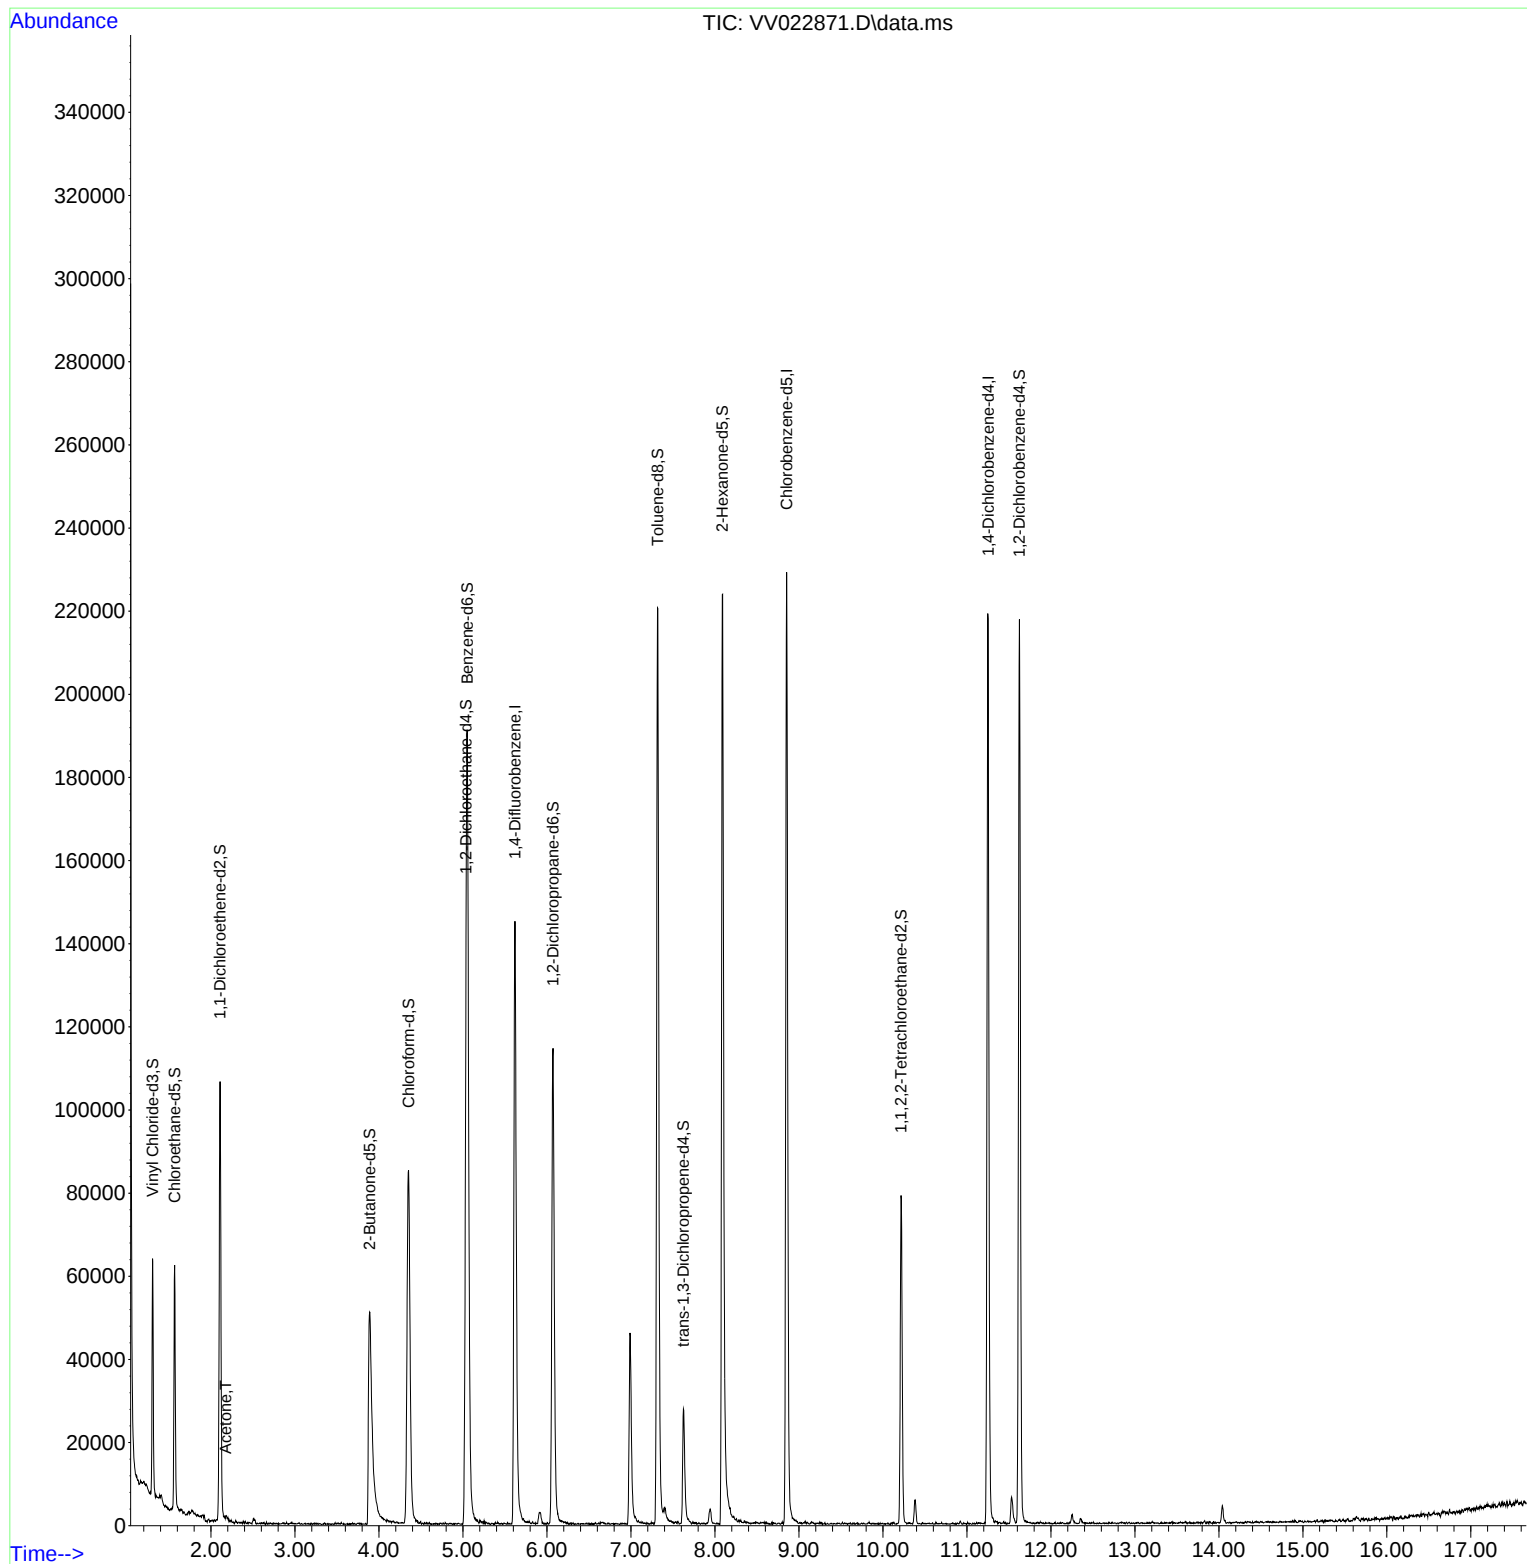

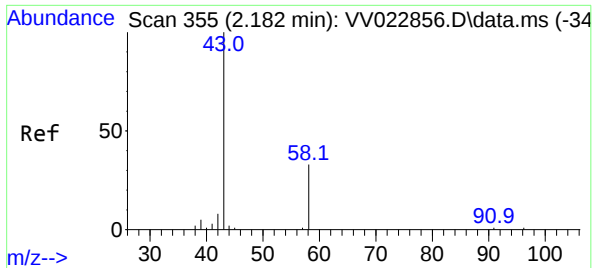

#13
 Acetone
 Concen: 1.16 ug/L
 RT: 2.175 min Scan# 353
 Delta R.T. -0.006 min
 Lab File: VV022871.D
 Acq: 18 Oct 2021 17:04

Instrument :
 MSVOA_V
 ClientSampleId :
 YAT53

Tgt Ion: 43 Resp: 1504
 Ion Ratio Lower Upper
 43 100
 58 33.9 0.0 24.2#

