

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
 Data File : VV022882.D
 Acq On : 18 Oct 2021 21:51
 Operator : SY/MD
 Sample : VV1018WBL02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK227

Quant Time: Oct 19 04:07:44 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 19 04:07:06 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	106792	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	108545	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	54489	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	35582	4.84	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	96.80%
7) Chloroethane-d5	1.568	69	32561	4.93	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.60%
11) 1,1-Dichloroethene-d2	2.108	63	54332	3.77	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.40%
20) 2-Butanone-d5	3.892	46	75891	39.39	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	78.78%
24) Chloroform-d	4.352	84	76206	5.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.60%
26) 1,2-Dichloroethane-d4	5.037	65	36994	5.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.60%
32) Benzene-d6	5.053	84	150763	4.67	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.40%
36) 1,2-Dichloropropane-d6	6.069	67	45596	4.76	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.20%
41) Toluene-d8	7.320	98	132640	4.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.00%
43) trans-1,3-Dichloroprop...	7.629	79	14739	4.64	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.80%
46) 2-Hexanone-d5	8.088	63	63256	49.45	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.90%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	32442	5.00	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.00%
66) 1,2-Dichlorobenzene-d4	11.625	152	54659	5.41	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.20%
Target Compounds						
13) Acetone	2.182	43	4048	3.77	ug/L	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022882.D
Acq On : 18 Oct 2021 21:51
Operator : SY/MD
Sample : VV1018WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK227

Quant Time: Oct 19 04:07:44 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 19 04:07:06 2021
Response via : Initial Calibration

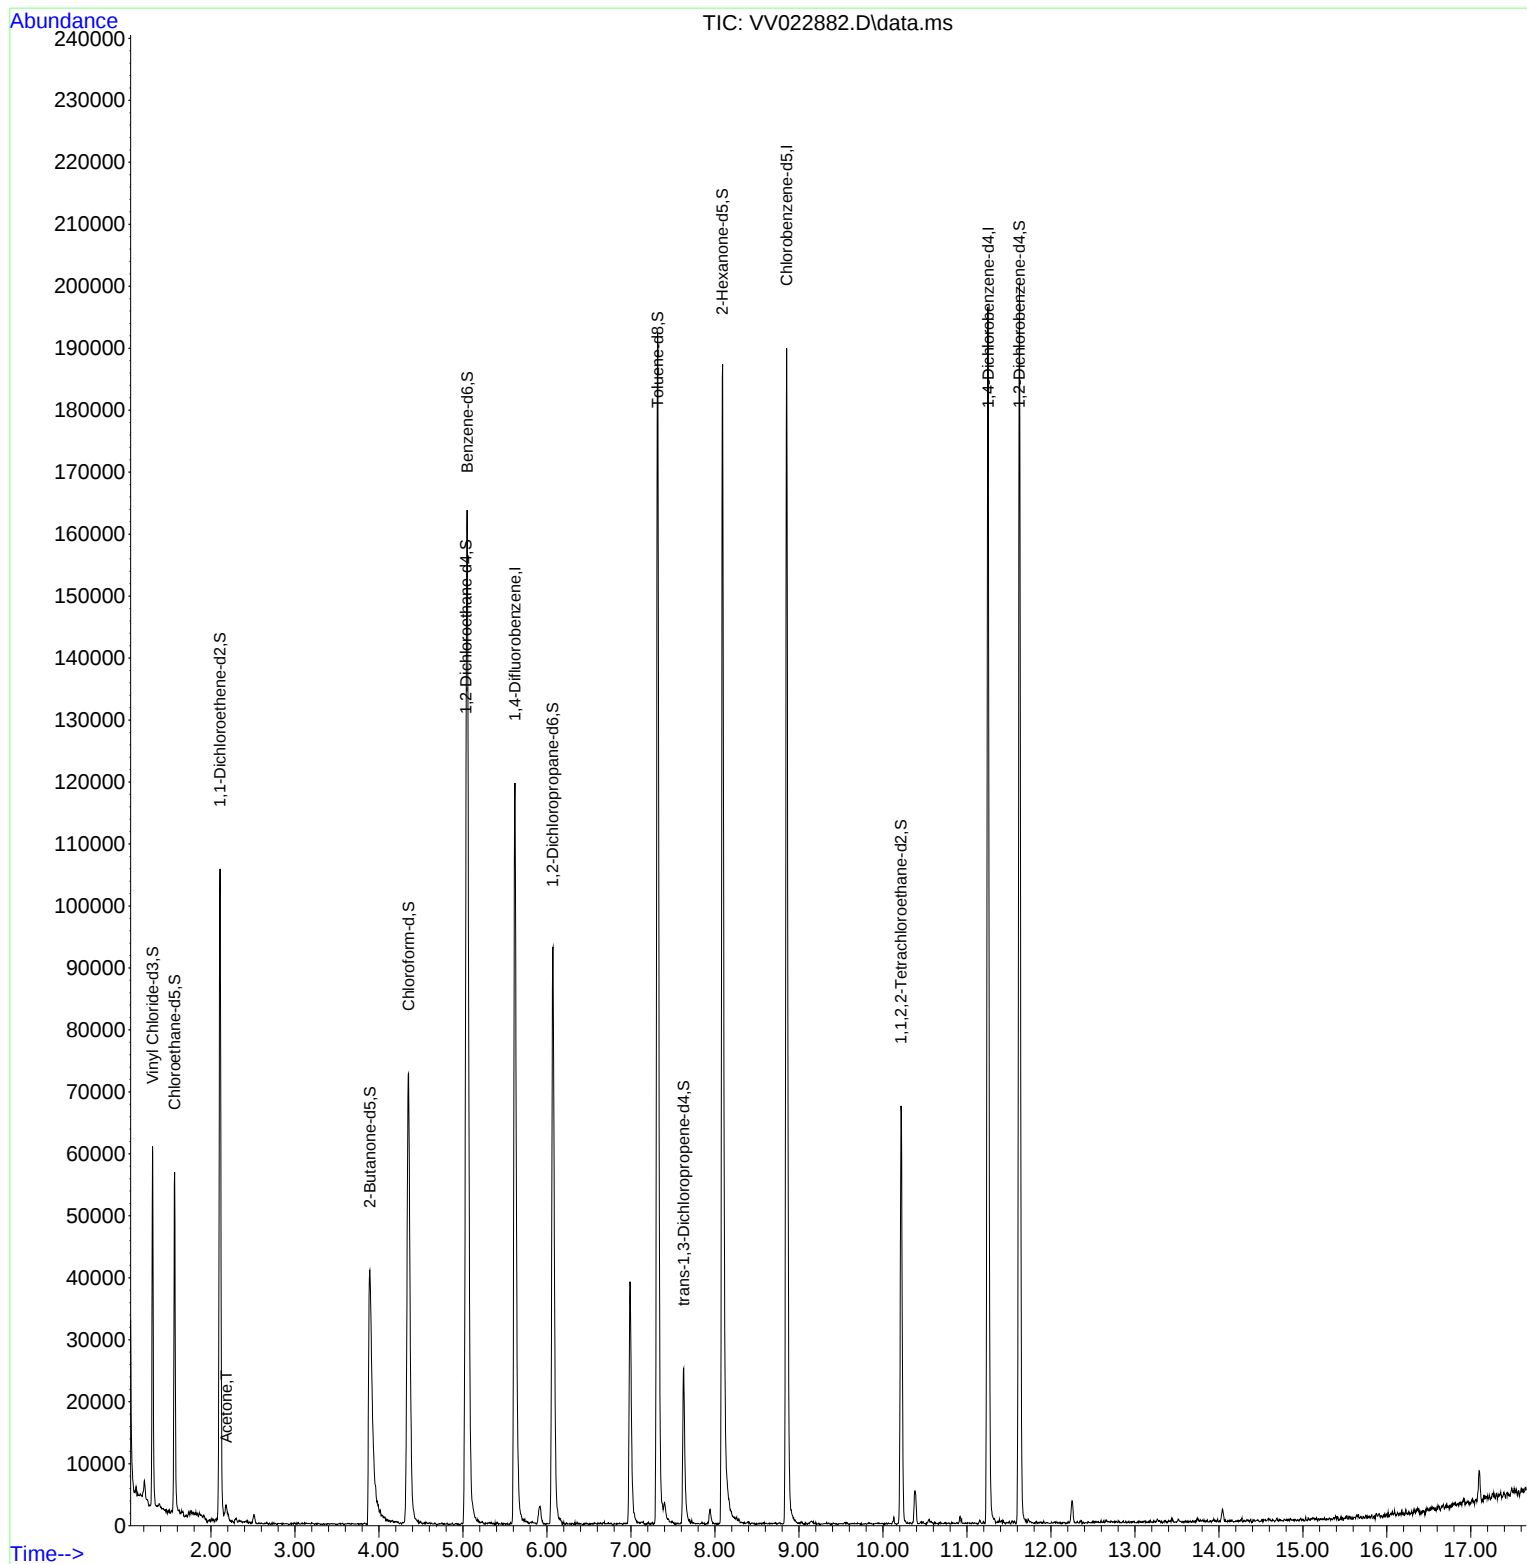

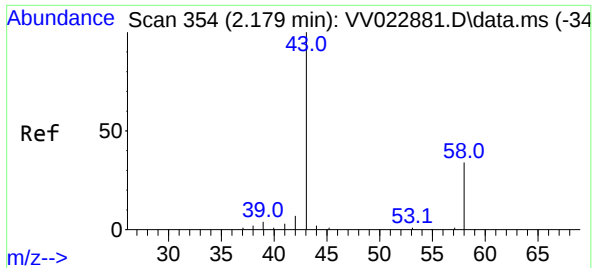

#13
Acetone
Concen: 3.77 ug/L
RT: 2.182 min Scan# 355
Delta R.T. 0.003 min
Lab File: VV022882.D
Acq: 18 Oct 2021 21:51

Instrument :
MSVOA_V
ClientSampleId :
VBLK227

Tgt Ion: 43 Resp: 4048
Ion Ratio Lower Upper
43 100
58 13.7 0.0 24.2

