

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
 Data File : VV022864.D
 Acq On : 18 Oct 2021 14:18
 Operator : SY/MD
 Sample : M4214-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022864.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	96	rVB	61304	61188	14.70%	1.836%
2	1.564	155	163	176	rBV	52526	61019	14.66%	1.831%
3	2.105	319	331	344	rBV	106488	156497	37.59%	4.696%
4	2.506	446	456	468	rBV2	11900	19692	4.73%	0.591%
5	3.908	882	892	921	rBV	22678	83069	19.95%	2.493%
6	4.352	1013	1030	1052	rBV	73768	183194	44.01%	5.497%
7	5.050	1230	1247	1280	rBV2	166363	416292	100.00%	12.492%
8	5.619	1411	1424	1445	rBV2	115252	234084	56.23%	7.024%
9	6.072	1549	1565	1589	rBV2	96228	196756	47.26%	5.904%
10	6.989	1840	1850	1868	rBV	42808	79751	19.16%	2.393%
11	7.317	1941	1952	1972	rBV	219024	386567	92.86%	11.600%
12	7.625	2039	2048	2067	rBV2	25390	48687	11.70%	1.461%
13	7.944	2137	2147	2156	rBV3	3581	6177	1.48%	0.185%
14	8.095	2180	2194	2221	rBV	152463	320981	77.10%	9.632%
15	8.853	2419	2430	2454	rBV	201235	331987	79.75%	9.962%
16	10.220	2842	2855	2873	rBV	70024	114045	27.40%	3.422%
17	10.387	2898	2907	2916	rVB4	4531	7597	1.82%	0.228%
18	11.249	3165	3175	3191	rBV	187330	295924	71.09%	8.880%
19	11.625	3280	3292	3310	rBV	210359	329005	79.03%	9.873%




Sum of corrected areas: 3332512

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022864.D
Acq On : 18 Oct 2021 14:18
Operator : SY/MD
Sample : M4214-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

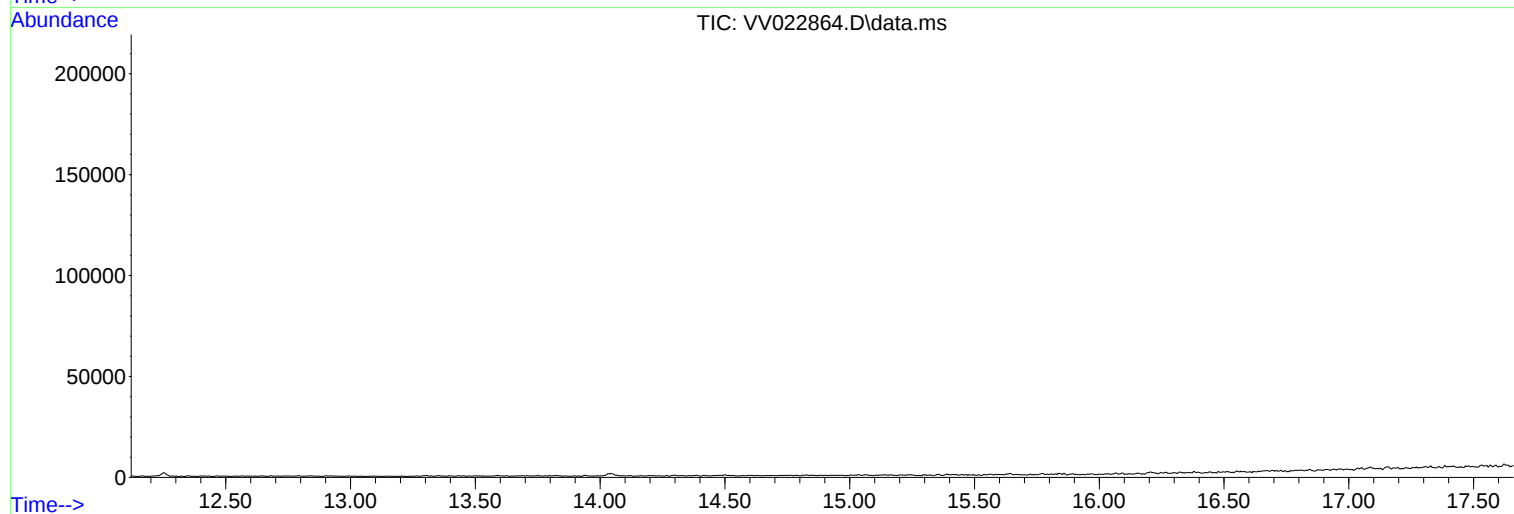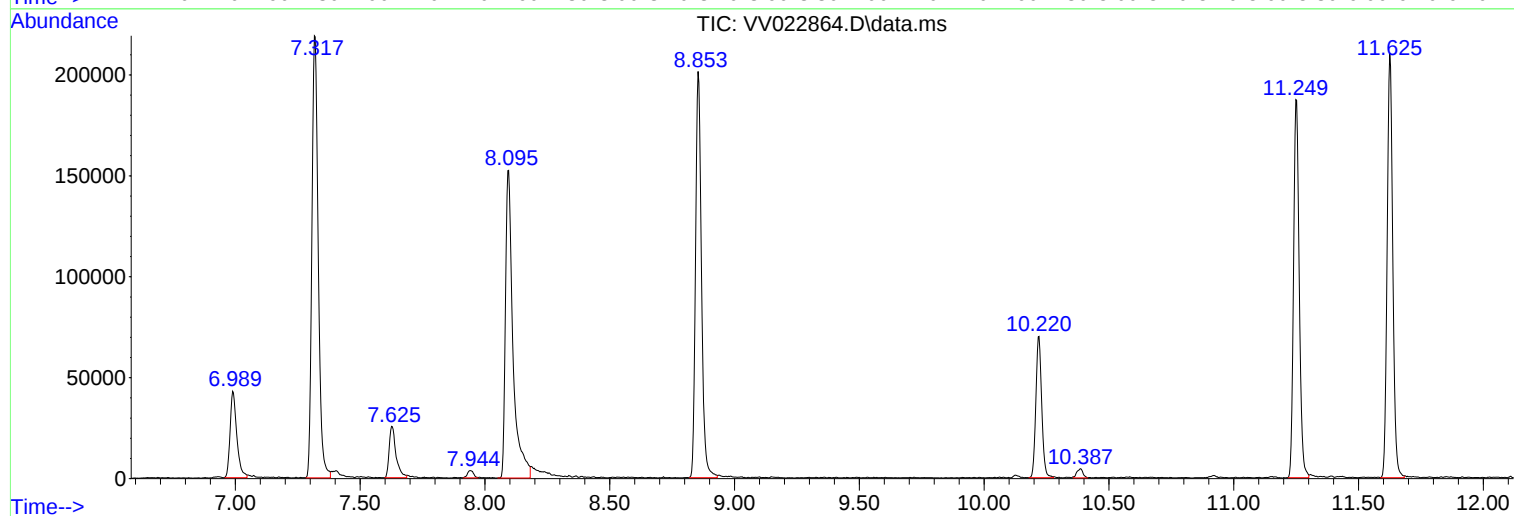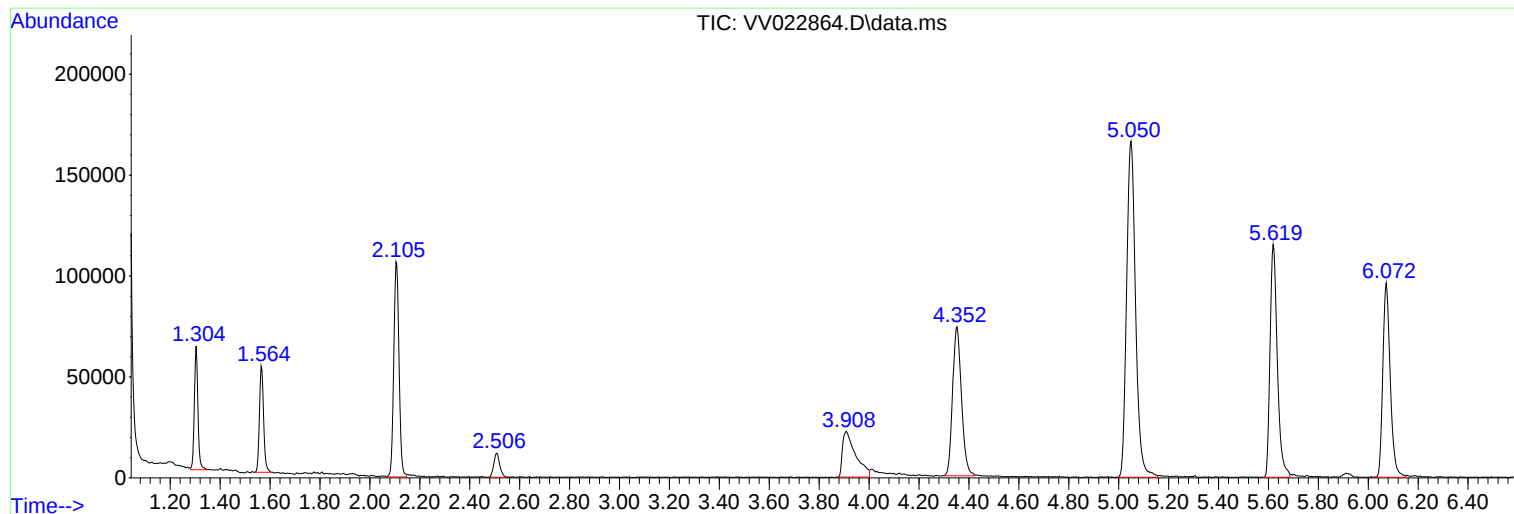

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022864.D
Acq On : 18 Oct 2021 14:18
Operator : SY/MD
Sample : M4214-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022864.D
Acq On : 18 Oct 2021 14:18
Operator : SY/MD
Sample : M4214-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
