

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
 Data File : VV022867.D
 Acq On : 18 Oct 2021 15:28
 Operator : SY/MD
 Sample : M4246-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YAT51

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022867.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	95	rVB	63030	63083	12.75%	1.604%
2	1.568	157	164	174	rBV	54847	61279	12.39%	1.558%
3	2.111	322	333	353	rBV	103541	154455	31.22%	3.927%
4	3.895	877	888	930	rBV	54745	187265	37.85%	4.762%
5	4.355	1015	1031	1055	rBV	87942	222392	44.95%	5.655%
6	5.053	1227	1248	1278	rBV3	193030	494706	100.00%	12.579%
7	5.622	1414	1425	1448	rBV	134754	275915	55.77%	7.016%
8	6.072	1552	1565	1587	rBV	115784	241037	48.72%	6.129%
9	6.992	1840	1851	1868	rBV	48001	89512	18.09%	2.276%
10	7.320	1941	1953	1970	rBV	224239	390183	78.87%	9.921%
11	7.397	1975	1977	1992	rVB5	3713	5935	1.20%	0.151%
12	7.628	2040	2049	2063	rBV2	28625	52201	10.55%	1.327%
13	7.944	2137	2147	2158	rVB3	3175	5528	1.12%	0.141%
14	8.091	2181	2193	2215	rBV	257950	462944	93.58%	11.771%
15	8.853	2418	2430	2454	rBV	216219	357064	72.18%	9.079%
16	10.217	2841	2854	2873	rBV	88767	139441	28.19%	3.546%
17	10.387	2897	2907	2915	rVB3	5061	8228	1.66%	0.209%
18	11.249	3165	3175	3196	rBV	215145	332555	67.22%	8.456%
19	11.535	3255	3264	3281	rBV3	13276	23720	4.79%	0.603%
20	11.625	3281	3292	3316	rVB	235812	365425	73.87%	9.292%




Sum of corrected areas: 3932868

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022867.D
Acq On : 18 Oct 2021 15:28
Operator : SY/MD
Sample : M4246-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAT51

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

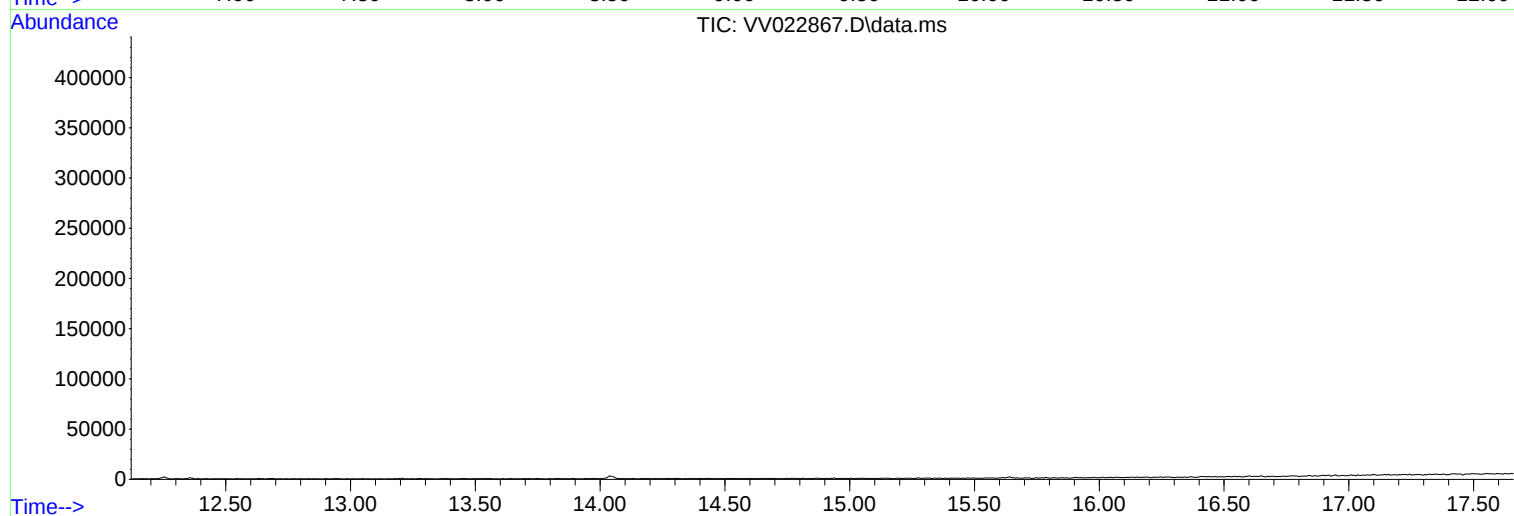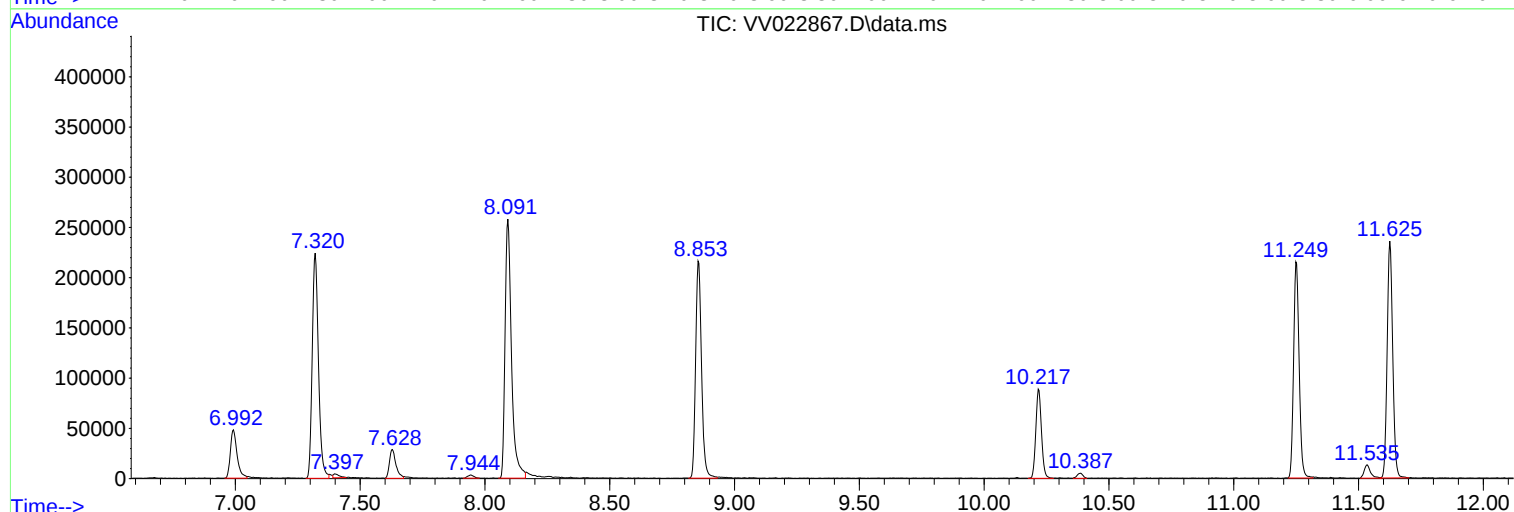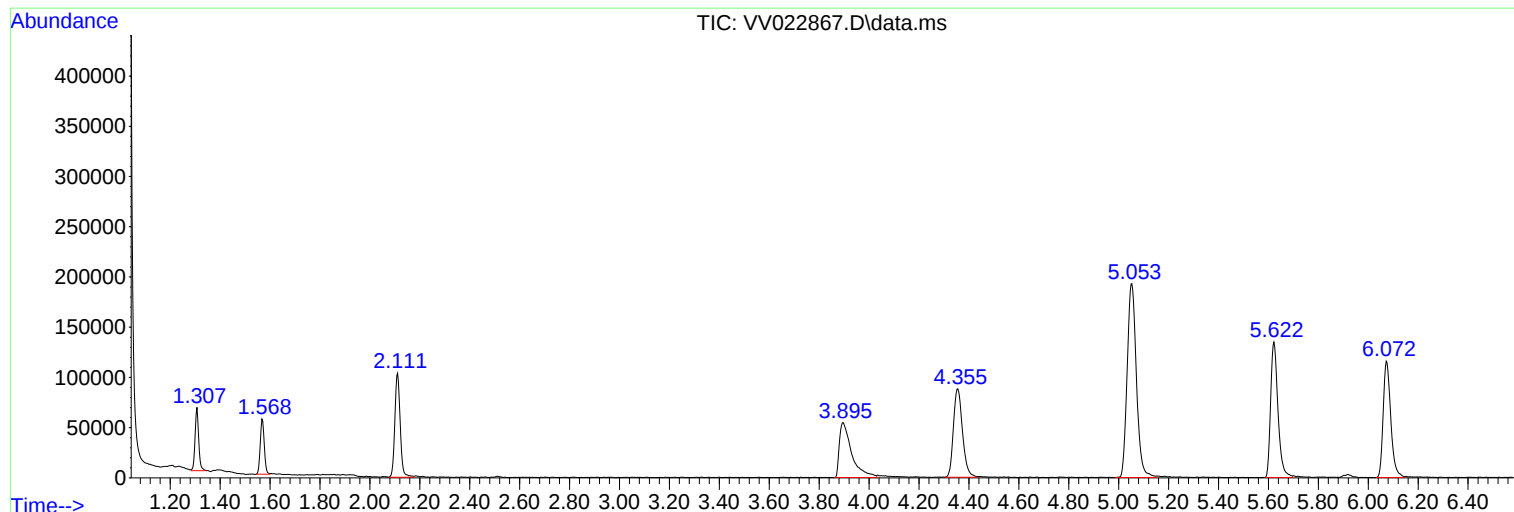

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022867.D
Acq On : 18 Oct 2021 15:28
Operator : SY/MD
Sample : M4246-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAT51

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022867.D
Acq On : 18 Oct 2021 15:28
Operator : SY/MD
Sample : M4246-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAT51

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
