

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
 Data File : VV022870.D
 Acq On : 18 Oct 2021 16:40
 Operator : SY/MD
 Sample : M4246-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YAT27

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022870.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	95	rVB	64544	68075	13.27%	1.714%
2	1.568	157	164	175	rBV	63035	70280	13.70%	1.770%
3	2.108	322	332	346	rBV	111253	161939	31.56%	4.078%
4	3.153	644	657	673	rBV2	9498	21373	4.17%	0.538%
5	3.896	877	888	922	rBV2	48285	173528	33.82%	4.370%
6	4.352	1014	1030	1046	rBV2	91508	225650	43.98%	5.682%
7	5.050	1230	1247	1277	rBV2	204797	513089	100.00%	12.920%
8	5.619	1412	1424	1455	rBV	134263	275919	53.78%	6.948%
9	6.072	1551	1565	1586	rBV	120998	249736	48.67%	6.289%
10	6.992	1840	1851	1875	rBV	49135	94364	18.39%	2.376%
11	7.317	1941	1952	1971	rBV	231007	413195	80.53%	10.405%
12	7.625	2039	2048	2063	rBV2	29561	52286	10.19%	1.317%
13	7.947	2134	2148	2160	rBV4	4380	8027	1.56%	0.202%
14	8.092	2183	2193	2221	rBV	245949	442966	86.33%	11.155%
15	8.854	2418	2430	2452	rBV	210330	351909	68.59%	8.862%
16	10.217	2843	2854	2868	rBV	88444	139500	27.19%	3.513%
17	10.384	2897	2906	2919	rVB3	6063	10024	1.95%	0.252%
18	11.249	3161	3175	3199	rBV	208995	324524	63.25%	8.172%
19	11.625	3279	3292	3315	rBV	237816	374742	73.04%	9.437%




Sum of corrected areas: 3971126

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022870.D
Acq On : 18 Oct 2021 16:40
Operator : SY/MD
Sample : M4246-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAT27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

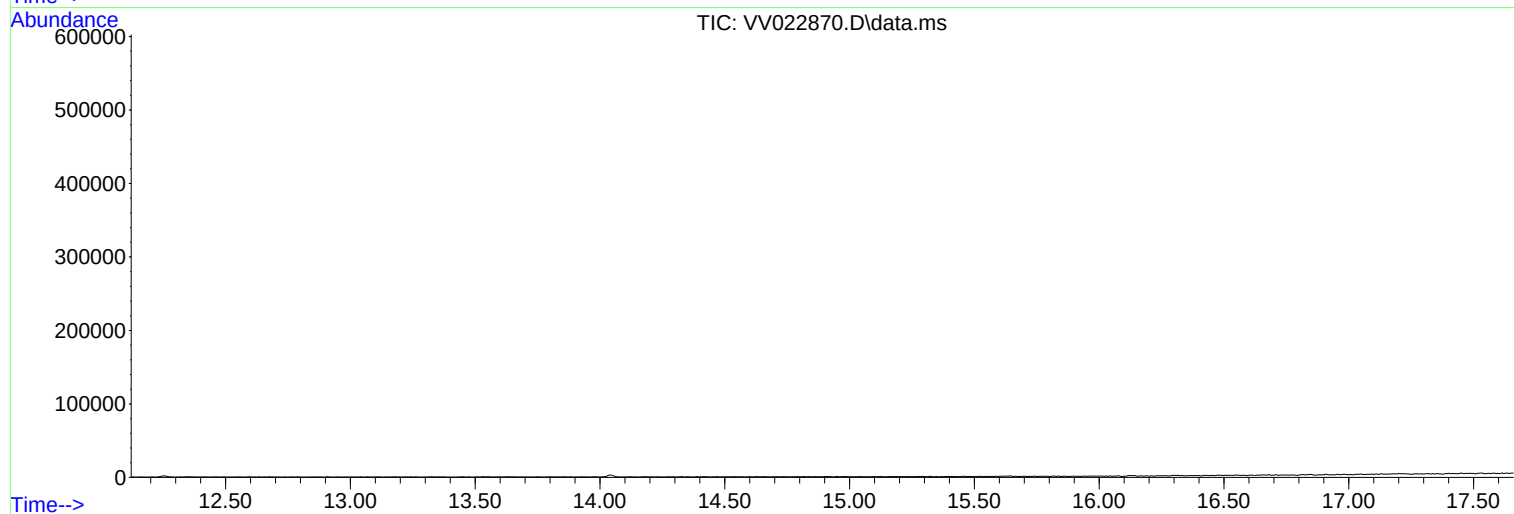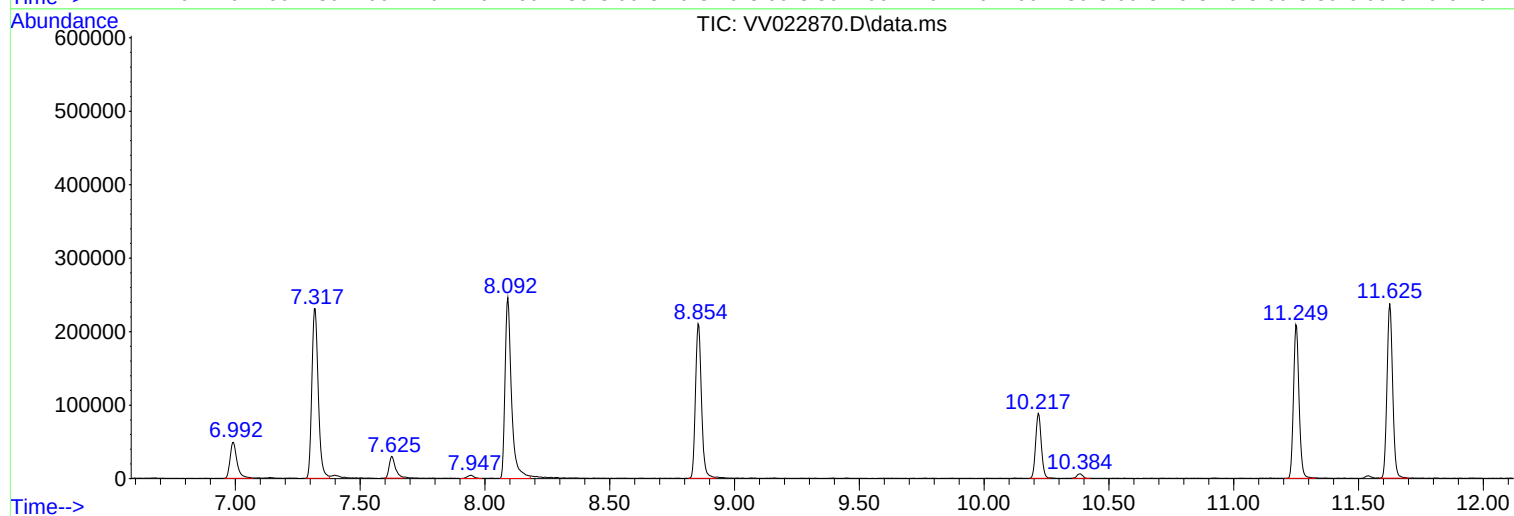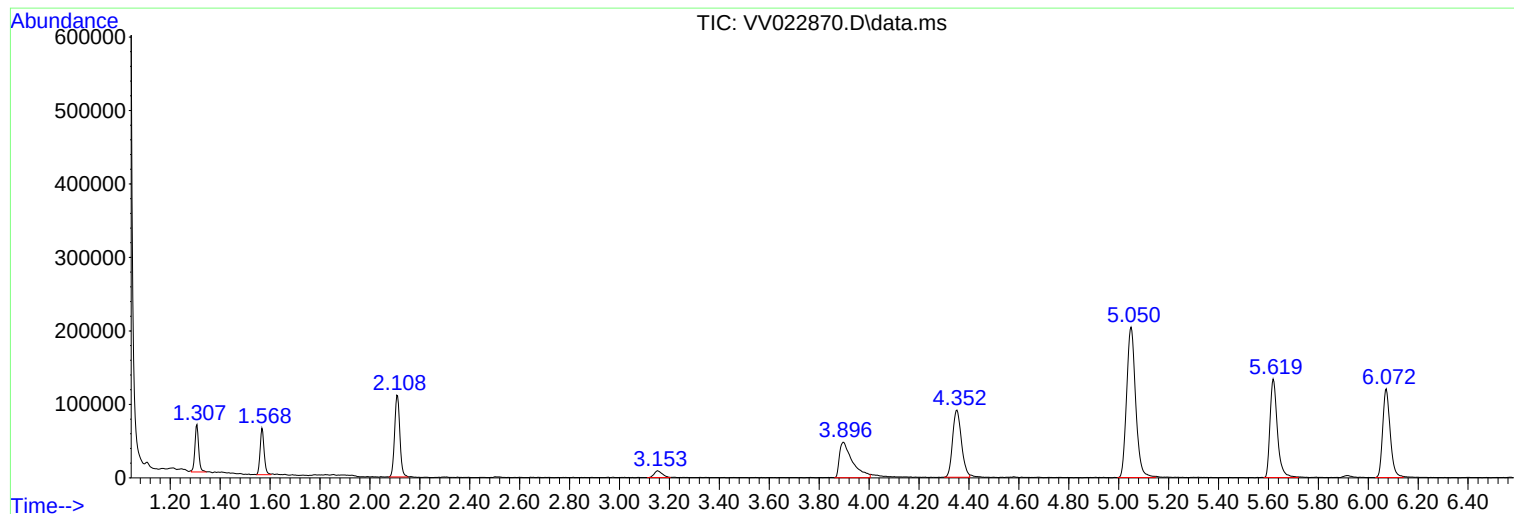

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022870.D
Acq On : 18 Oct 2021 16:40
Operator : SY/MD
Sample : M4246-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAT27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022870.D
Acq On : 18 Oct 2021 16:40
Operator : SY/MD
Sample : M4246-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAT27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
