

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
 Data File : VV022871.D
 Acq On : 18 Oct 2021 17:04
 Operator : SY/MD
 Sample : M4246-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YAT53

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022871.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	93	rVB	57435	59637	12.48%	1.563%
2	1.568	157	164	181	rVB	59178	68881	14.41%	1.805%
3	2.108	322	332	346	rBV	105498	151793	31.76%	3.978%
4	3.889	876	886	926	rBV2	51143	164076	34.33%	4.299%
5	4.352	1014	1030	1054	rBV	84878	214809	44.95%	5.629%
6	5.050	1231	1247	1275	rBV2	191082	477904	100.00%	12.523%
7	5.619	1412	1424	1452	rBV	144975	295257	61.78%	7.737%
8	6.072	1549	1565	1588	rBV	114537	234814	49.13%	6.153%
9	6.989	1840	1850	1867	rBV	46061	86437	18.09%	2.265%
10	7.317	1941	1952	1972	rBV	220309	386191	80.81%	10.120%
11	7.625	2039	2048	2065	rBV	27507	49464	10.35%	1.296%
12	7.944	2136	2147	2157	rVB2	3511	6158	1.29%	0.161%
13	8.091	2183	2193	2220	rBV	223746	407748	85.32%	10.685%
14	8.853	2418	2430	2451	rBV	229034	373484	78.15%	9.787%
15	10.217	2843	2854	2874	rVB	78952	125089	26.17%	3.278%
16	10.384	2897	2906	2919	rBV2	5832	9124	1.91%	0.239%
17	11.249	3165	3175	3192	rBV	218860	341676	71.49%	8.953%
18	11.532	3255	3263	3277	rBV4	6378	11613	2.43%	0.304%
19	11.625	3281	3292	3313	rVV	217248	345767	72.35%	9.060%
20	14.040	4034	4043	4051	rBV	4166	6289	1.32%	0.165%




Sum of corrected areas: 3816211

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022871.D
Acq On : 18 Oct 2021 17:04
Operator : SY/MD
Sample : M4246-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAT53

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

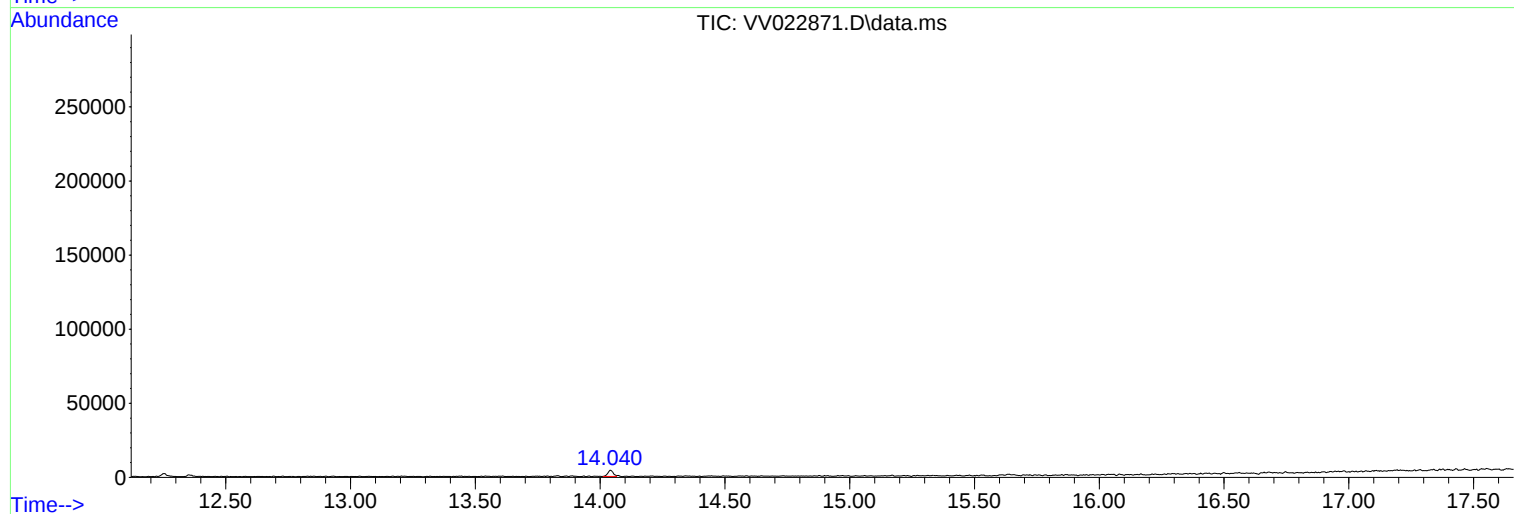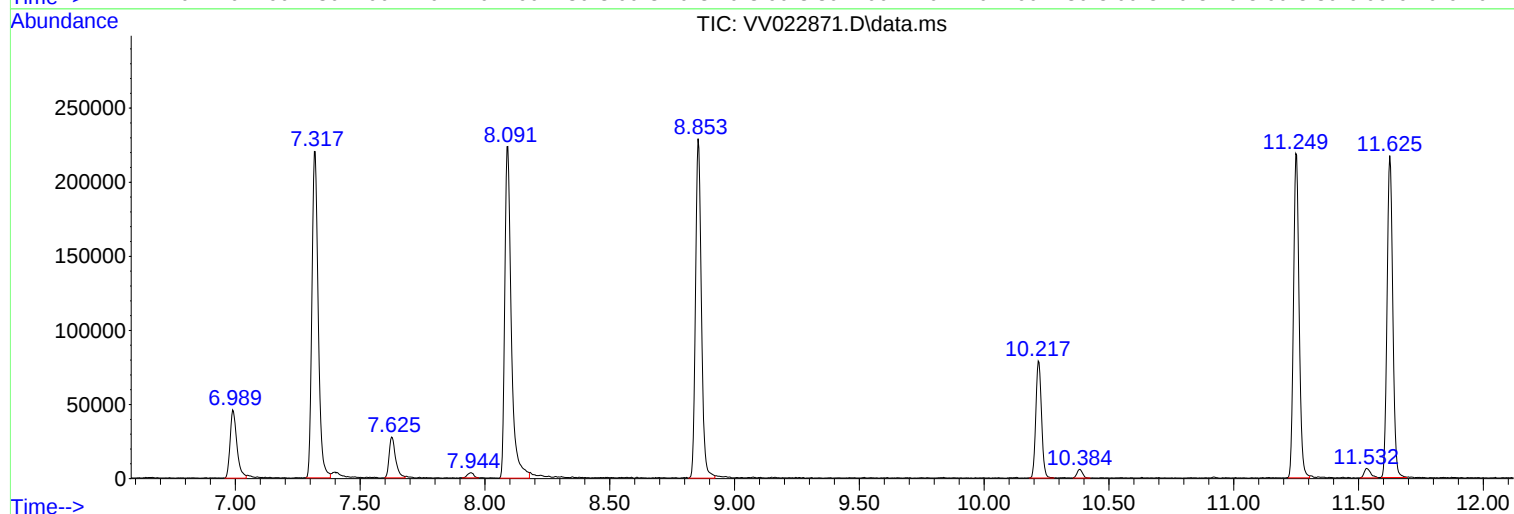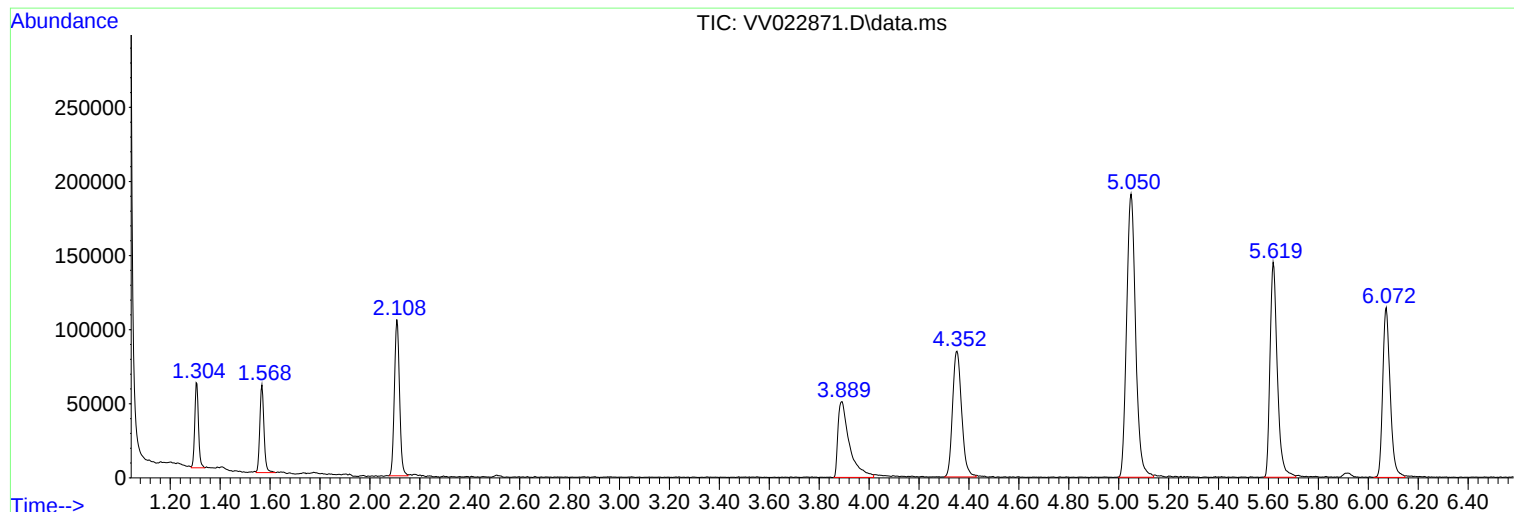

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022871.D
Acq On : 18 Oct 2021 17:04
Operator : SY/MD
Sample : M4246-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAT53

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022871.D
Acq On : 18 Oct 2021 17:04
Operator : SY/MD
Sample : M4246-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAT53

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
