

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
 Data File : VV022875.D
 Acq On : 18 Oct 2021 18:39
 Operator : SY/MD
 Sample : M4200-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGD7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022875.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	96	rVB2	66103	73065	17.57%	1.799%
2	1.568	156	164	177	rVB	48348	55977	13.46%	1.378%
3	2.108	318	332	346	rBV	88492	130527	31.39%	3.213%
4	2.510	446	457	468	rVB3	2889	4921	1.18%	0.121%
5	2.770	526	538	553	rBV2	11953	25294	6.08%	0.623%
6	3.192	657	669	689	rVB	17133	35532	8.55%	0.875%
7	3.909	877	892	921	rBV2	99165	316165	76.04%	7.783%
8	4.352	1014	1030	1058	rBV3	76258	203107	48.85%	5.000%
9	5.050	1231	1247	1274	rBV2	165075	415789	100.00%	10.235%
10	5.619	1411	1424	1447	rBV	122468	245115	58.95%	6.034%
11	5.921	1505	1518	1539	rBV5	20774	45951	11.05%	1.131%
12	6.072	1552	1565	1587	rBV	97661	200938	48.33%	4.946%
13	6.989	1840	1850	1872	rBV	39973	76950	18.51%	1.894%
14	7.317	1940	1952	1971	rBV	197799	346151	83.25%	8.521%
15	7.400	1972	1978	1995	rVB2	6711	11826	2.84%	0.291%
16	7.625	2039	2048	2072	rBV2	25645	46699	11.23%	1.150%
17	7.976	2139	2157	2178	rBV	120074	212495	51.11%	5.231%
18	8.092	2182	2193	2226	rBV	216125	391777	94.22%	9.644%
19	8.854	2419	2430	2451	rBV	213521	359014	86.35%	8.837%
20	9.149	2513	2522	2529	rBV4	2663	4414	1.06%	0.109%
21	10.217	2844	2854	2870	rBV	84690	135208	32.52%	3.328%
22	10.384	2893	2906	2919	rVB4	7698	13061	3.14%	0.322%
23	11.098	3117	3128	3136	rVB4	3068	4588	1.10%	0.113%
24	11.252	3164	3176	3194	rVV	219072	338614	81.44%	8.335%
25	11.625	3279	3292	3313	rBV	228404	358910	86.32%	8.835%
26	12.252	3476	3487	3495	rBV4	3440	5883	1.41%	0.145%
27	14.040	4036	4043	4054	rBV2	2639	4481	1.08%	0.110%


Sum of corrected areas: 4062452

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022875.D
Acq On : 18 Oct 2021 18:39
Operator : SY/MD
Sample : M4200-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGD7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

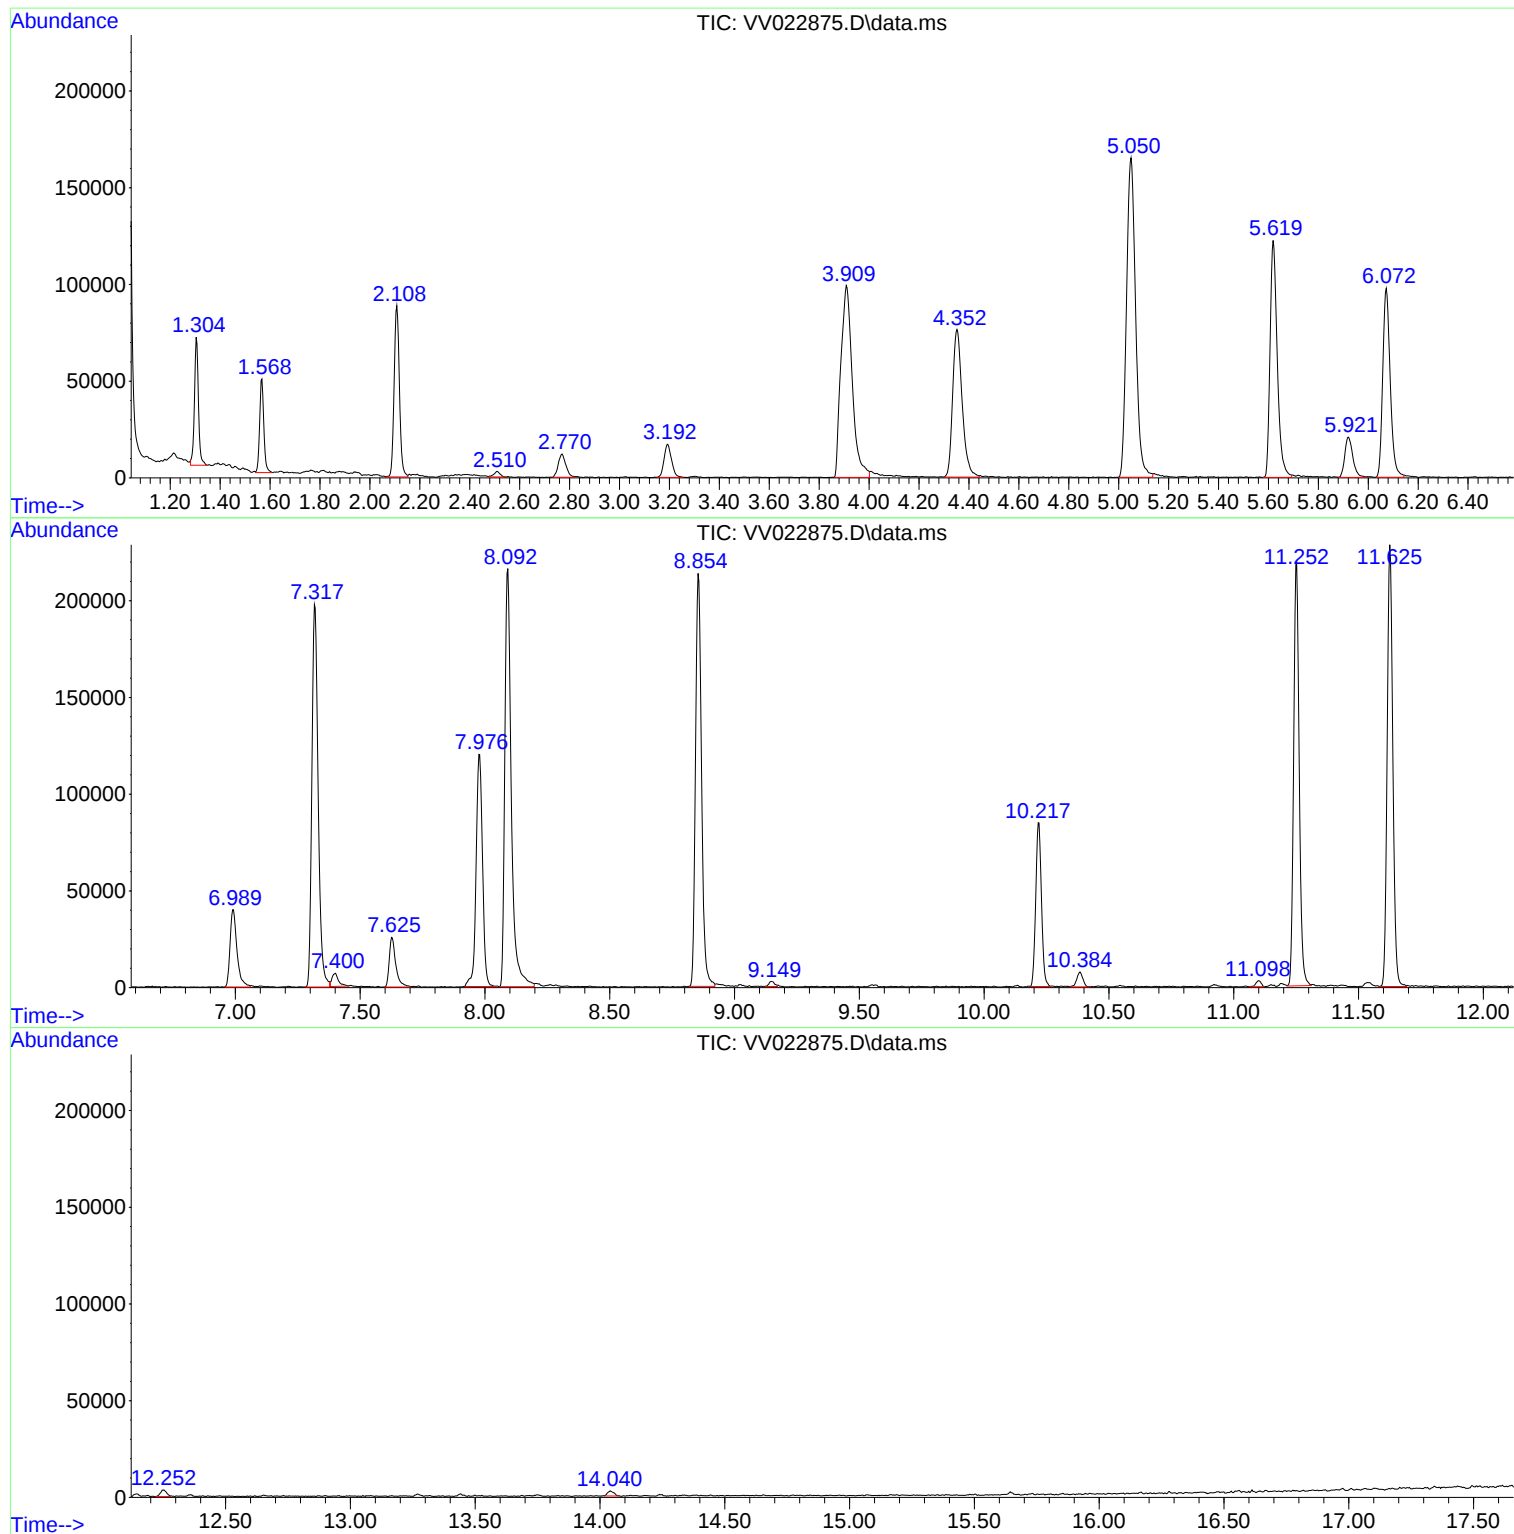

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022875.D
Acq On : 18 Oct 2021 18:39
Operator : SY/MD
Sample : M4200-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGD7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022875.D
Acq On : 18 Oct 2021 18:39
Operator : SY/MD
Sample : M4200-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGD7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
