

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
 Data File : VV022876.D
 Acq On : 18 Oct 2021 19:03
 Operator : SY/MD
 Sample : M4200-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFG3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022876.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	95	rVB2	77933	87101	1.97%	0.968%
2	1.565	156	163	176	rBV	56881	66176	1.50%	0.736%
3	2.105	322	331	344	rBV	104251	152430	3.45%	1.695%
4	2.182	344	355	383	rBV	90421	257751	5.83%	2.866%
5	2.365	392	412	449	rBV2	36167	245299	5.55%	2.727%
6	3.909	876	892	937	rBV	1827857	4422066	100.00%	49.169%
7	4.352	1014	1030	1055	rVB2	88083	221289	5.00%	2.461%
8	5.050	1230	1247	1268	rBV2	198207	491827	11.12%	5.469%
9	5.619	1412	1424	1447	rBV	133705	272084	6.15%	3.025%
10	6.072	1551	1565	1592	rBV2	115732	240373	5.44%	2.673%
11	6.989	1840	1850	1873	rBV	48306	90572	2.05%	1.007%
12	7.317	1940	1952	1965	rBV	222381	390417	8.83%	4.341%
13	7.391	1965	1975	1994	rVB	181011	317238	7.17%	3.527%
14	7.625	2040	2048	2063	rBV	28678	51109	1.16%	0.568%
15	8.092	2183	2193	2228	rBV	223219	458541	10.37%	5.099%
16	8.854	2414	2430	2452	rBV	212406	350993	7.94%	3.903%
17	10.217	2843	2854	2873	rBV	88019	140251	3.17%	1.559%
18	11.249	3165	3175	3196	rVB	209595	348264	7.88%	3.872%
19	11.625	3279	3292	3310	rBV	238351	389860	8.82%	4.335%




Sum of corrected areas: 8993641

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022876.D
Acq On : 18 Oct 2021 19:03
Operator : SY/MD
Sample : M4200-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGE3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

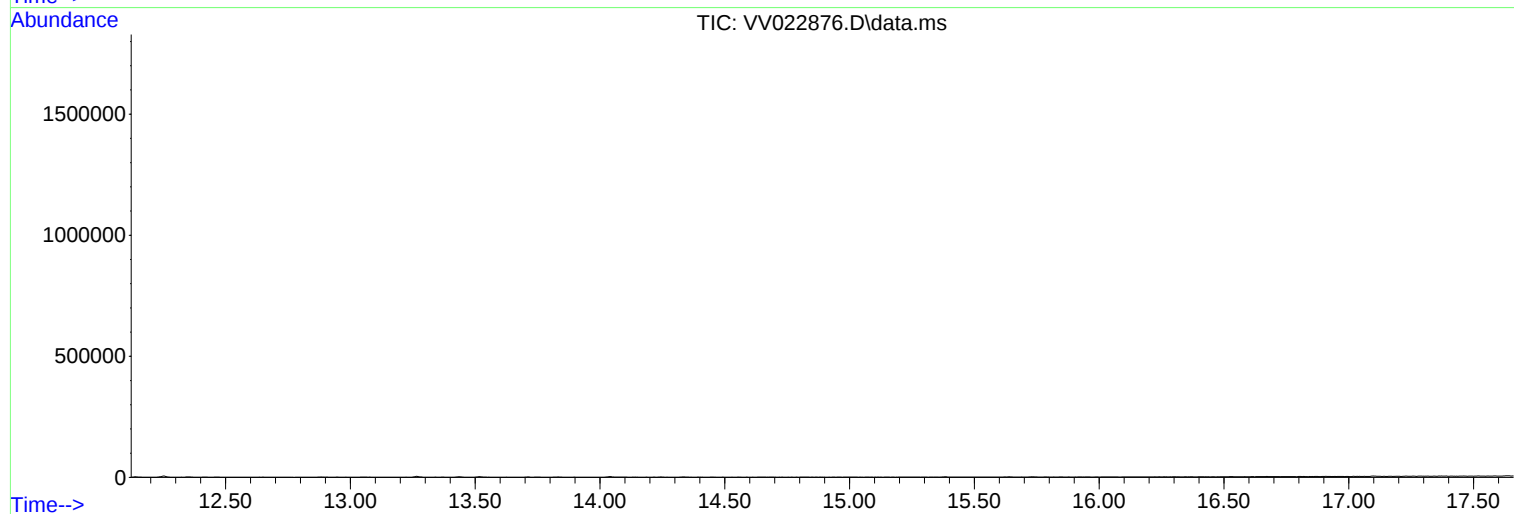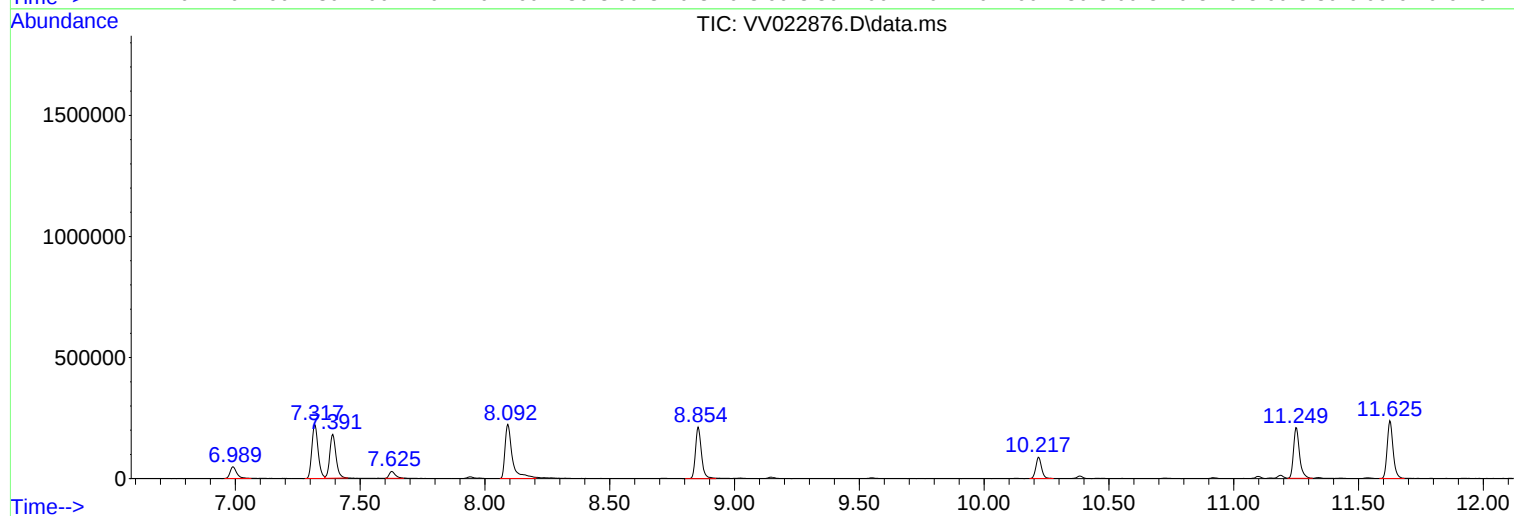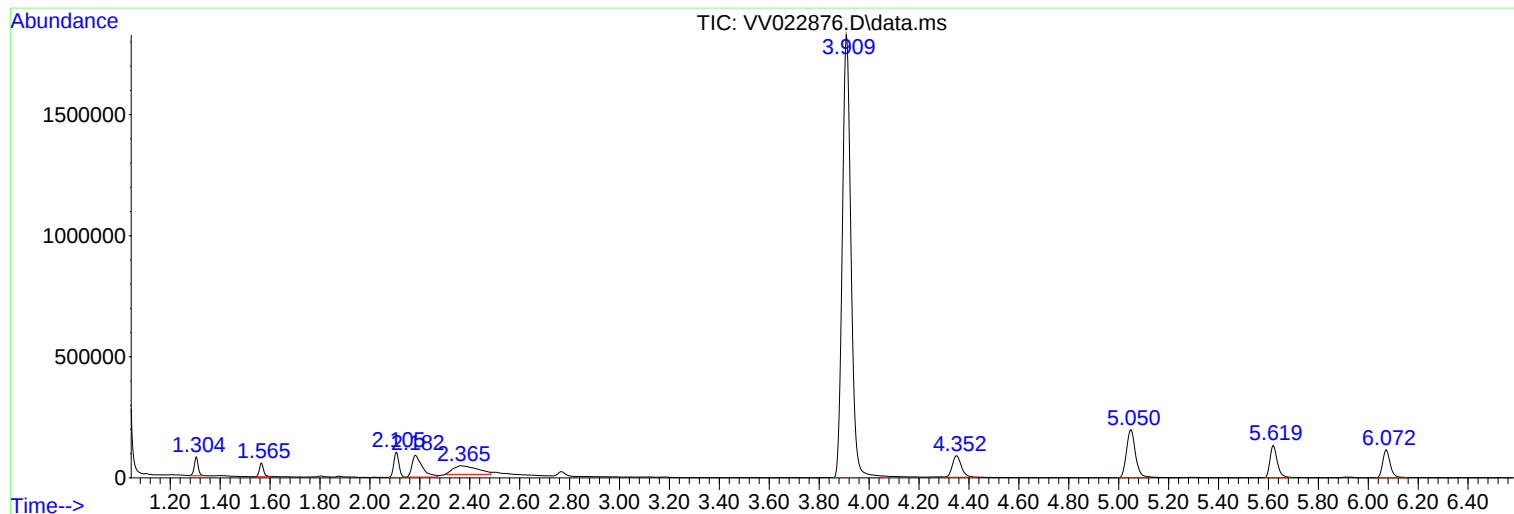

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022876.D
Acq On : 18 Oct 2021 19:03
Operator : SY/MD
Sample : M4200-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGE3










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.365	4.51 ug/L	245299	1,4-Difluorobenzene	5.619

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	80
2			Isopropyl Alcohol	60	C3H8O	000067-63-0	72
3			Isopropyl Alcohol	60	C3H8O	000067-63-0	56
4			Isopropyl Alcohol	60	C3H8O	000067-63-0	9
5			L-Lactic acid	90	C3H6O3	000079-33-4	9

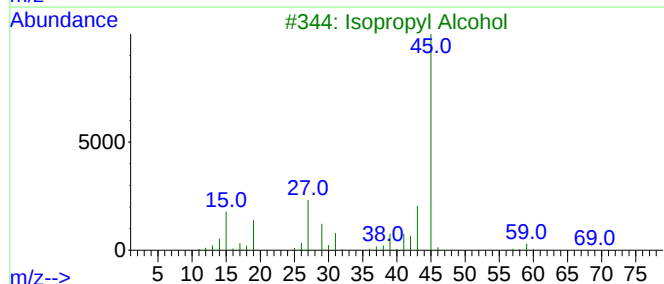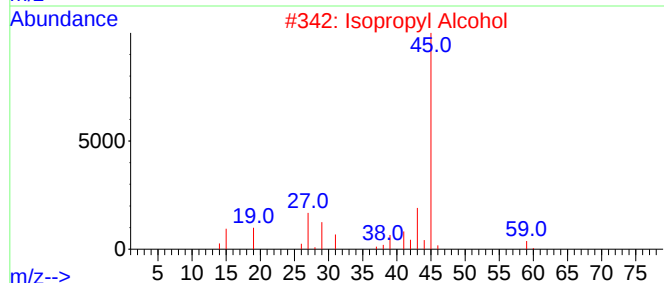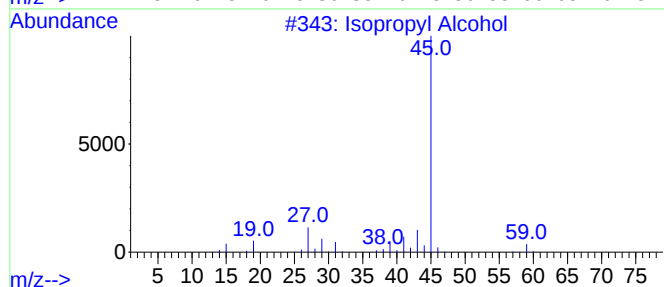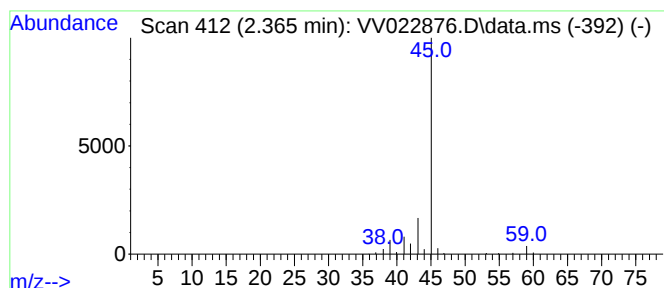

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022876.D
Acq On : 18 Oct 2021 19:03
Operator : SY/MD
Sample : M4200-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGE3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.365	4.5	ug/L	245299	1	5.619	272084	5.0