

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
 Data File : VV022877.D
 Acq On : 18 Oct 2021 19:27
 Operator : SY/MD
 Sample : M4200-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGE4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022877.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	92	rBV2	69391	74803	2.89%	1.047%
2	1.568	156	164	173	rBV	46620	55718	2.15%	0.780%
3	2.108	321	332	343	rBV	102757	146781	5.68%	2.054%
4	2.188	344	357	383	rBV	50035	166865	6.45%	2.335%
5	2.394	386	421	422	rBV6	77108	301032	11.64%	4.212%
6	2.764	526	536	556	rVB4	37167	77143	2.98%	1.079%
7	3.908	876	892	931	rBV	1041643	2585596	100.00%	36.177%
8	4.352	1012	1030	1056	rVB	87581	222665	8.61%	3.115%
9	5.050	1231	1247	1287	rBV2	198152	501072	19.38%	7.011%
10	5.619	1413	1424	1448	rBV	135242	274512	10.62%	3.841%
11	6.072	1550	1565	1589	rBV2	114675	239710	9.27%	3.354%
12	6.992	1838	1851	1868	rBV	47074	88218	3.41%	1.234%
13	7.317	1940	1952	1965	rBV	221897	388636	15.03%	5.438%
14	7.391	1965	1975	2000	rVB	160099	284321	11.00%	3.978%
15	7.625	2039	2048	2068	rBV	28961	52757	2.04%	0.738%
16	8.091	2182	2193	2230	rBV	254022	470823	18.21%	6.588%
17	8.854	2419	2430	2448	rBV	211447	349729	13.53%	4.893%
18	10.220	2840	2855	2869	rBV	89599	139947	5.41%	1.958%
19	11.252	3166	3176	3197	rVB	214611	344624	13.33%	4.822%
20	11.625	3280	3292	3315	rVB	234815	382100	14.78%	5.346%




Sum of corrected areas: 7147052

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022877.D
Acq On : 18 Oct 2021 19:27
Operator : SY/MD
Sample : M4200-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGE4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

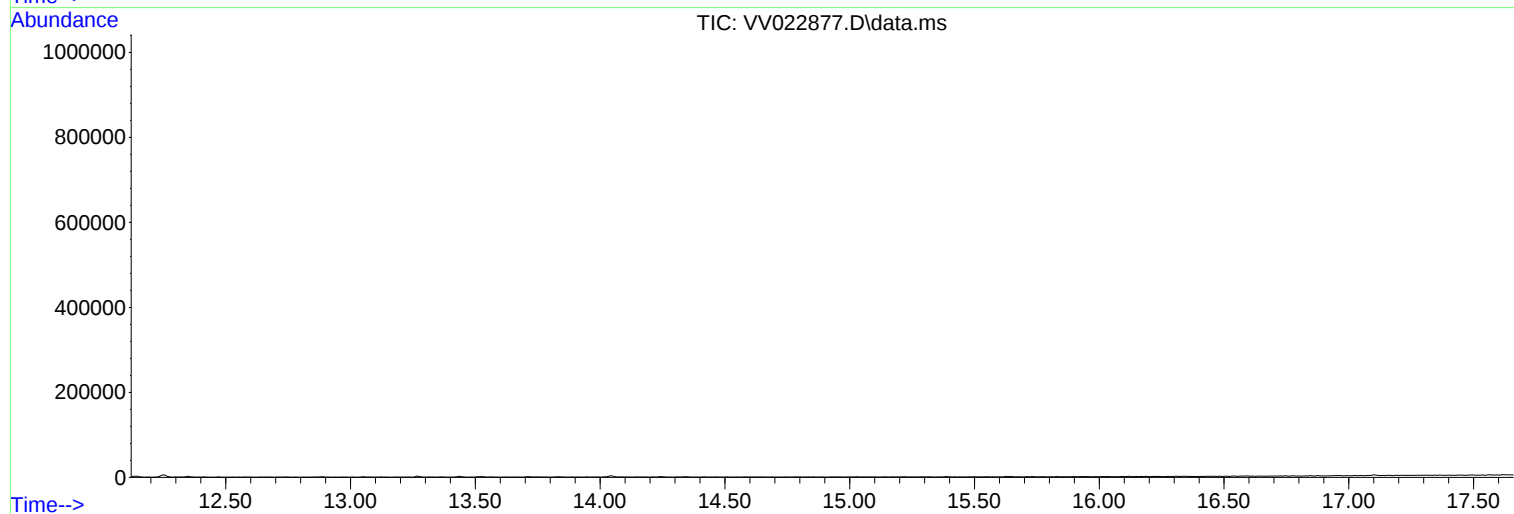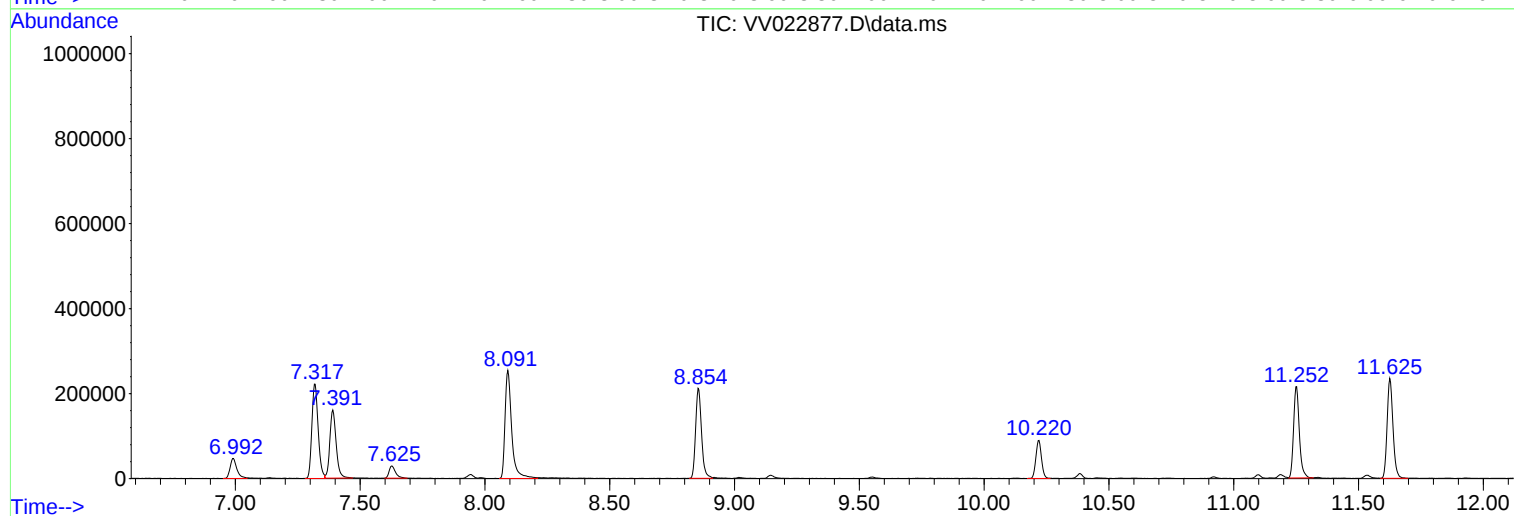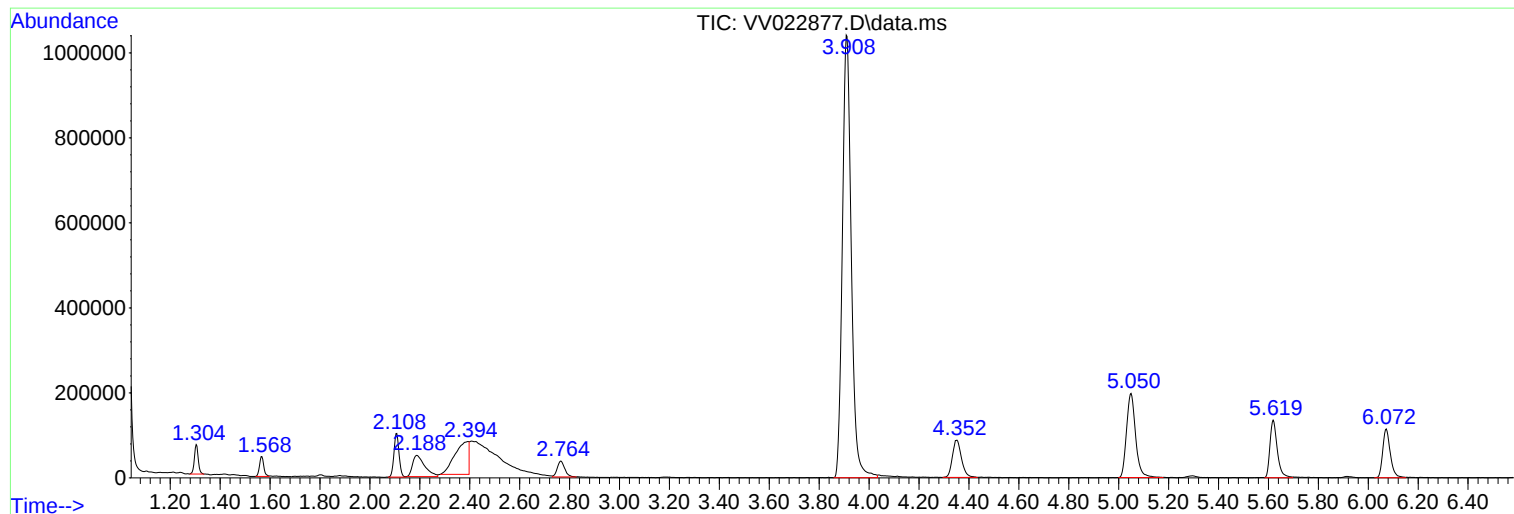

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022877.D
Acq On : 18 Oct 2021 19:27
Operator : SY/MD
Sample : M4200-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGE4










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.394	5.48 ug/L	301032	1,4-Difluorobenzene	5.619

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
2			Isopropyl Alcohol	60	C3H8O	000067-63-0	72
3			Isopropyl Alcohol	60	C3H8O	000067-63-0	72
4			Isopropyl Alcohol	60	C3H8O	000067-63-0	72
5			Isopropyl Alcohol	60	C3H8O	000067-63-0	56

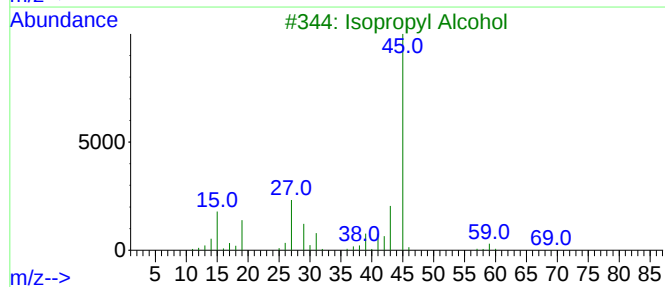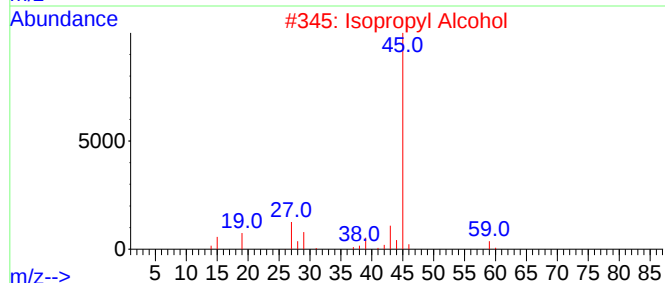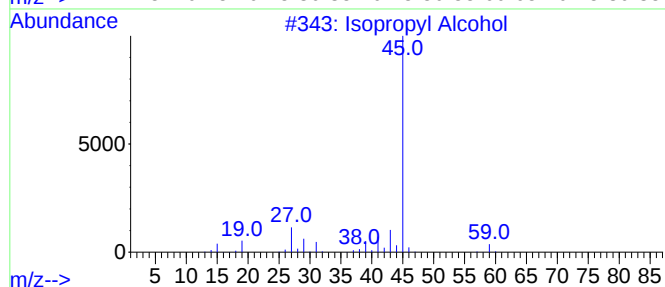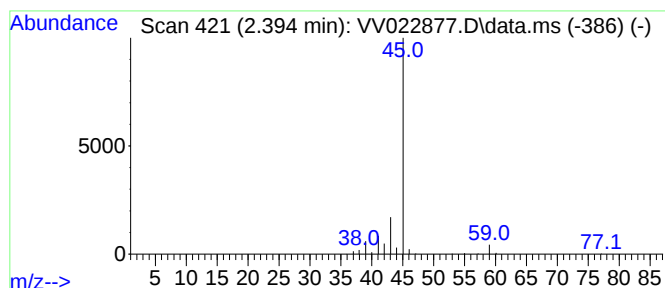

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022877.D
Acq On : 18 Oct 2021 19:27
Operator : SY/MD
Sample : M4200-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGE4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.394	5.5	ug/L	301032	1	5.619	274512	5.0