

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
 Data File : VV022882.D
 Acq On : 18 Oct 2021 21:51
 Operator : SY/MD
 Sample : VV1018WBL02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK227

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022882.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.208	49	52	69	rVB4	4117	6616	1.62%	0.201%
2	1.304	76	82	97	rVB	58051	58881	14.42%	1.789%
3	1.568	156	164	178	rBV	54801	61542	15.07%	1.870%
4	2.108	319	332	346	rBV	105209	152121	37.24%	4.622%
5	3.892	877	887	913	rBV	41118	127482	31.21%	3.873%
6	4.352	1013	1030	1056	rBV2	72468	180974	44.31%	5.498%
7	5.050	1230	1247	1284	rBV3	163577	408444	100.00%	12.409%
8	5.619	1410	1424	1451	rBV	119557	241533	59.13%	7.338%
9	5.918	1504	1517	1530	rBV5	2836	6479	1.59%	0.197%
10	6.072	1552	1565	1588	rBV	93014	190525	46.65%	5.789%
11	6.989	1839	1850	1865	rBV	39037	71023	17.39%	2.158%
12	7.317	1941	1952	1969	rBV	191982	338626	82.91%	10.288%
13	7.629	2040	2049	2069	rBV	24977	43602	10.68%	1.325%
14	8.092	2182	2193	2222	rBV	187045	337786	82.70%	10.263%
15	8.854	2419	2430	2454	rBV	189653	311356	76.23%	9.460%
16	10.217	2841	2854	2868	rBV	67441	106107	25.98%	3.224%
17	10.381	2898	2905	2918	rVB4	5330	9165	2.24%	0.278%
18	11.249	3165	3175	3198	rBV	196210	308764	75.60%	9.381%
19	11.625	3279	3292	3314	rBV	200149	316847	77.57%	9.627%
20	12.252	3477	3487	3496	rBV2	3597	5739	1.41%	0.174%
21	17.098	4986	4994	5003	rVB3	4996	7782	1.91%	0.236%


Sum of corrected areas: 3291394

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022882.D
Acq On : 18 Oct 2021 21:51
Operator : SY/MD
Sample : VV1018WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK227

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

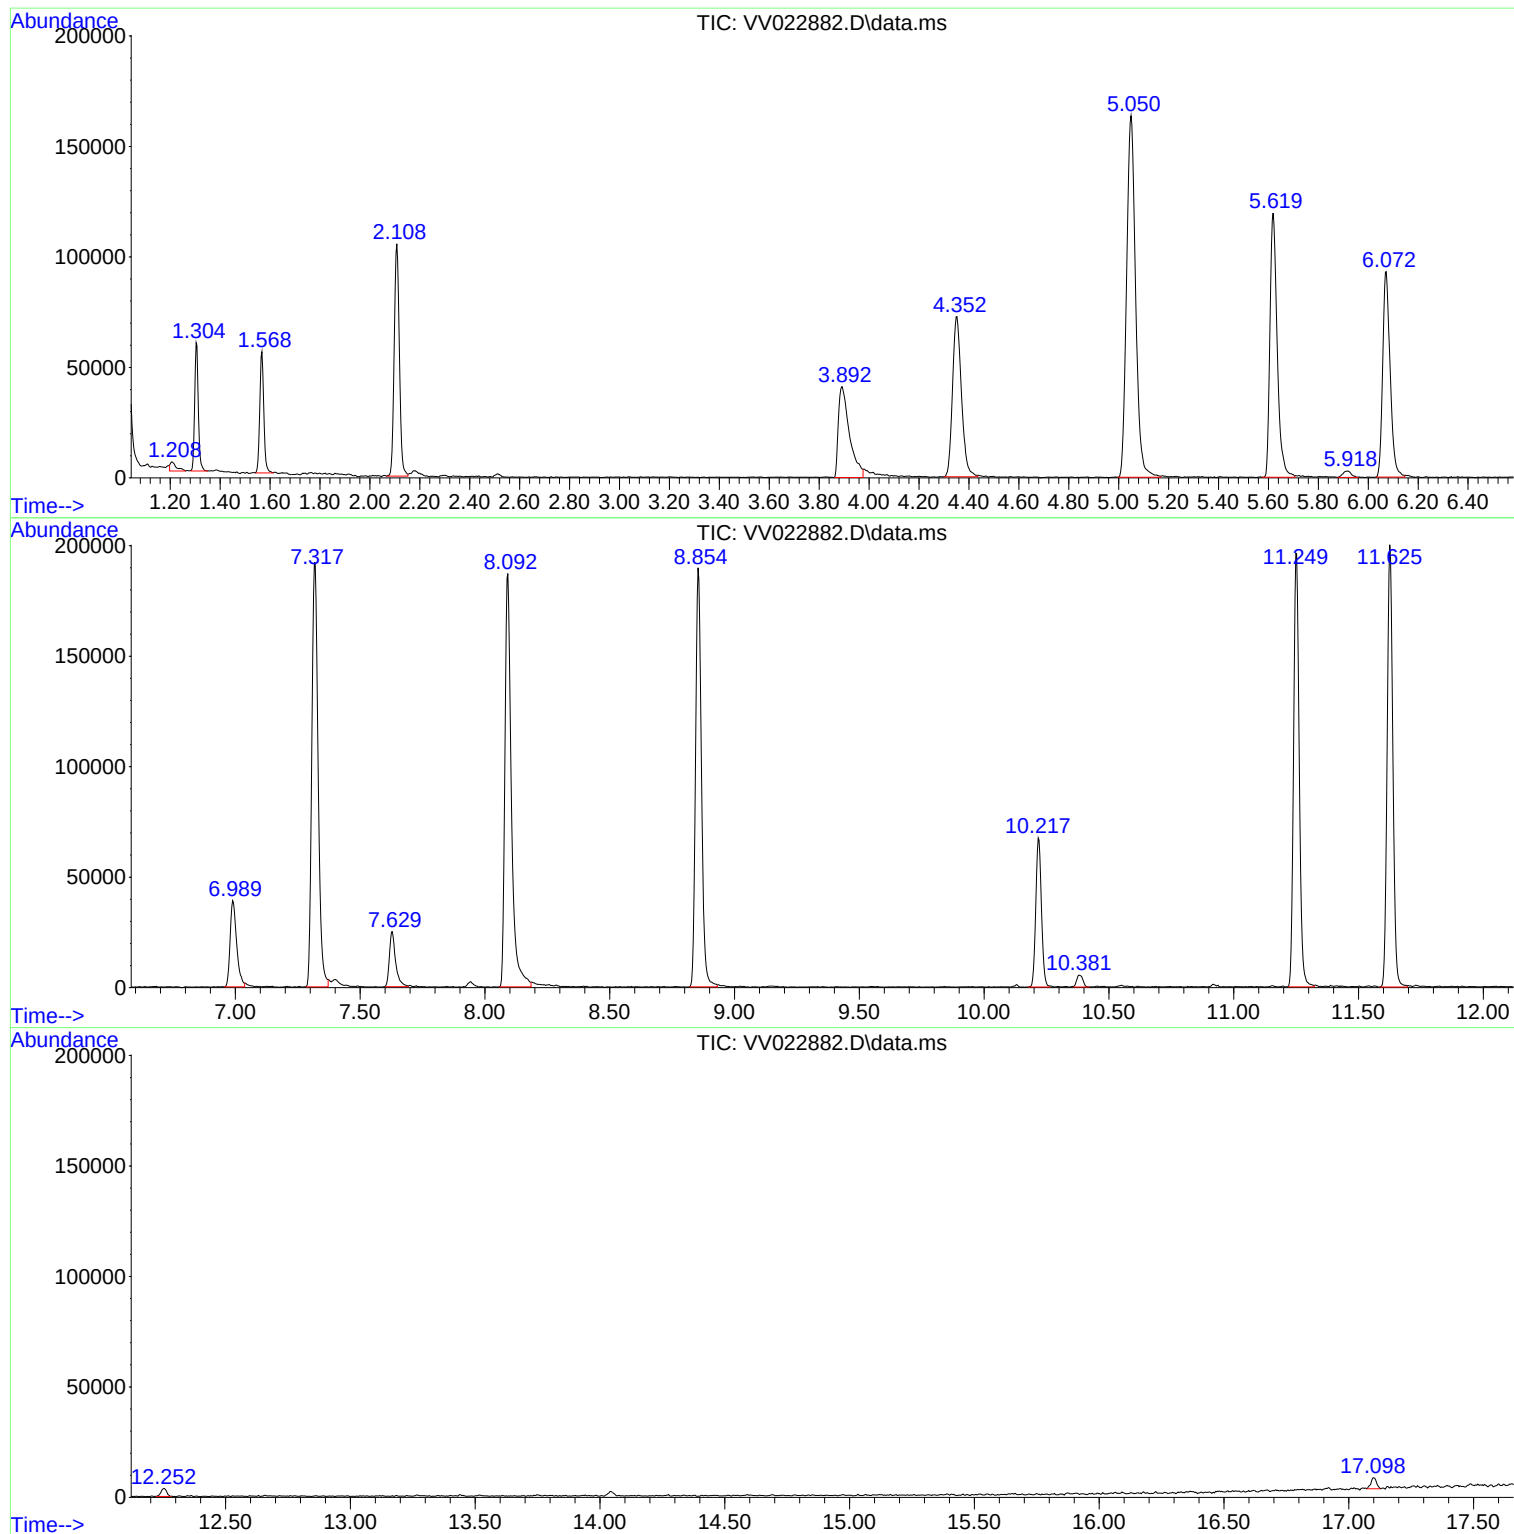

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022882.D
Acq On : 18 Oct 2021 21:51
Operator : SY/MD
Sample : VV1018WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK227

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022882.D
Acq On : 18 Oct 2021 21:51
Operator : SY/MD
Sample : VV1018WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK227

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
