

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
 Data File : VV022887.D
 Acq On : 18 Oct 2021 23:54
 Operator : SY/MD
 Sample : M4137-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFG91

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022887.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	97	rVB	57352	62966	7.73%	1.109%
2	1.568	156	164	176	rVB	52775	60484	7.43%	1.066%
3	2.108	322	332	351	rVB	93897	137924	16.94%	2.430%
4	3.915	878	894	939	rBV4	165818	504524	61.97%	8.888%
5	4.352	1012	1030	1065	rBV	89613	244304	30.01%	4.304%
6	5.050	1231	1247	1274	rBV2	194455	495524	60.86%	8.730%
7	5.619	1412	1424	1447	rBV	132616	272016	33.41%	4.792%
8	5.918	1505	1517	1536	rBV	63850	131460	16.15%	2.316%
9	6.072	1552	1565	1590	rBV2	113398	239620	29.43%	4.221%
10	6.989	1840	1850	1870	rBV2	46256	87517	10.75%	1.542%
11	7.317	1941	1952	1964	rBV	224195	387087	47.55%	6.819%
12	7.387	1964	1974	1995	rVB	474135	814147	100.00%	14.343%
13	7.628	2039	2049	2065	rBV2	28456	52406	6.44%	0.923%
14	7.976	2132	2157	2180	rBV	303152	521155	64.01%	9.181%
15	8.091	2183	2193	2219	rBV	264955	474978	58.34%	8.368%
16	8.853	2419	2430	2452	rBV	211565	348722	42.83%	6.144%
17	10.217	2841	2854	2867	rBV	87915	139202	17.10%	2.452%
18	10.384	2895	2906	2916	rBV2	6921	11471	1.41%	0.202%
19	11.249	3164	3175	3198	rBV	205876	317949	39.05%	5.601%
20	11.535	3256	3264	3276	rVB3	7364	12500	1.54%	0.220%
21	11.625	3276	3292	3312	rBV	227204	360288	44.25%	6.347%




Sum of corrected areas: 5676244

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022887.D
Acq On : 18 Oct 2021 23:54
Operator : SY/MD
Sample : M4137-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFG91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

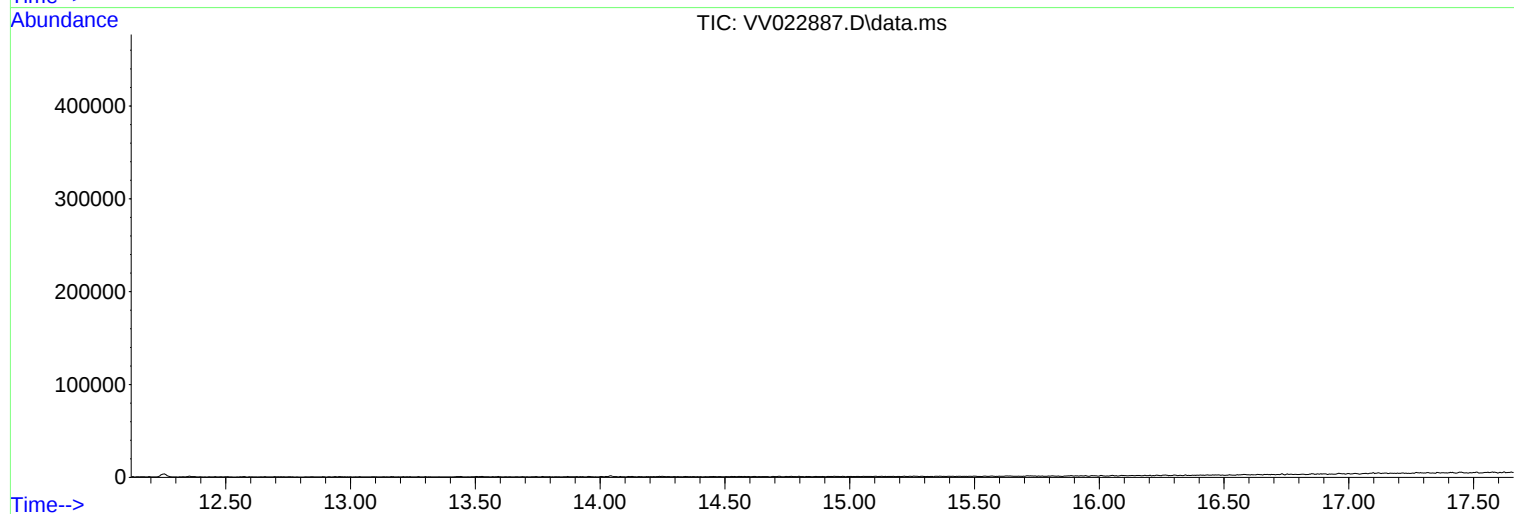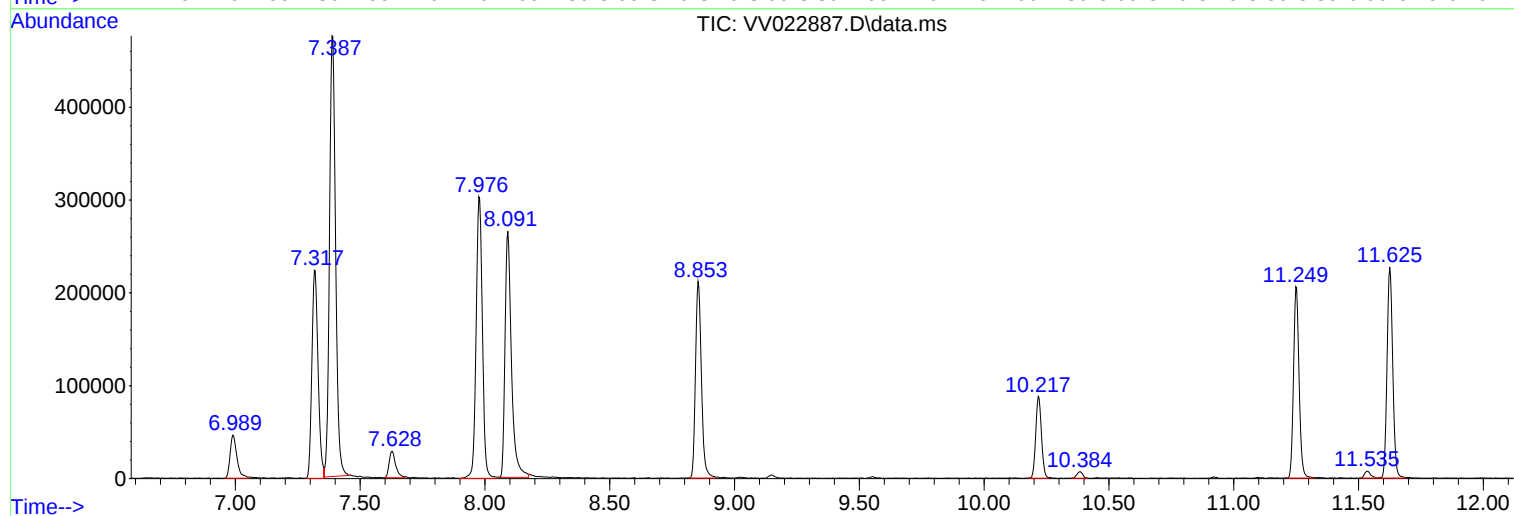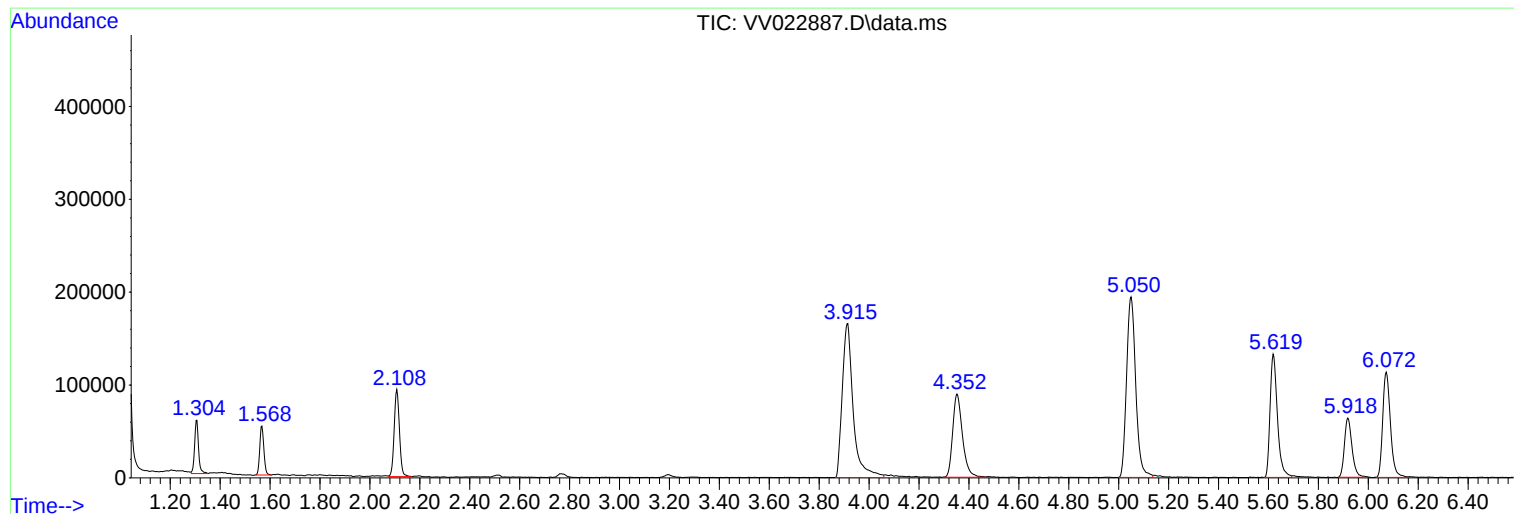

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022887.D
Acq On : 18 Oct 2021 23:54
Operator : SY/MD
Sample : M4137-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFG91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022887.D
Acq On : 18 Oct 2021 23:54
Operator : SY/MD
Sample : M4137-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFG91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
