

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
 Data File : VV022893.D
 Acq On : 19 Oct 2021 02:17
 Operator : SY/MD
 Sample : M4137-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGA9

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022893.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	95	rVB2	79262	85029	4.75%	1.311%
2	1.568	156	164	176	rBV	54196	63551	3.55%	0.980%
3	2.108	322	332	345	rVB2	101606	150514	8.41%	2.320%
4	2.764	525	536	553	rBV5	44222	86112	4.81%	1.328%
5	3.912	875	893	926	rBV2	699894	1790733	100.00%	27.608%
6	4.352	1013	1030	1056	rBV	84250	213416	11.92%	3.290%
7	5.050	1231	1247	1276	rBV2	189430	476945	26.63%	7.353%
8	5.619	1413	1424	1454	rBV	130987	270163	15.09%	4.165%
9	5.918	1504	1517	1540	rBV	75021	151425	8.46%	2.335%
10	6.072	1552	1565	1583	rBV2	108540	224486	12.54%	3.461%
11	6.989	1837	1850	1874	rBV	42703	83767	4.68%	1.291%
12	7.317	1941	1952	1967	rBV	213168	378946	21.16%	5.842%
13	7.391	1967	1975	1994	rVB	53335	98973	5.53%	1.526%
14	7.629	2039	2049	2066	rBV	27818	49444	2.76%	0.762%
15	7.976	2134	2157	2177	rBV	457424	787400	43.97%	12.139%
16	8.092	2183	2193	2220	rBV	225604	397145	22.18%	6.123%
17	8.854	2418	2430	2458	rBV	207701	349253	19.50%	5.384%
18	10.217	2842	2854	2871	rBV	78407	126590	7.07%	1.952%
19	10.384	2895	2906	2915	rBV2	13659	21676	1.21%	0.334%
20	11.249	3165	3175	3197	rVB	208145	332182	18.55%	5.121%
21	11.625	3281	3292	3315	rVB	209155	348533	19.46%	5.373%




Sum of corrected areas: 6486283

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022893.D
Acq On : 19 Oct 2021 02:17
Operator : SY/MD
Sample : M4137-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

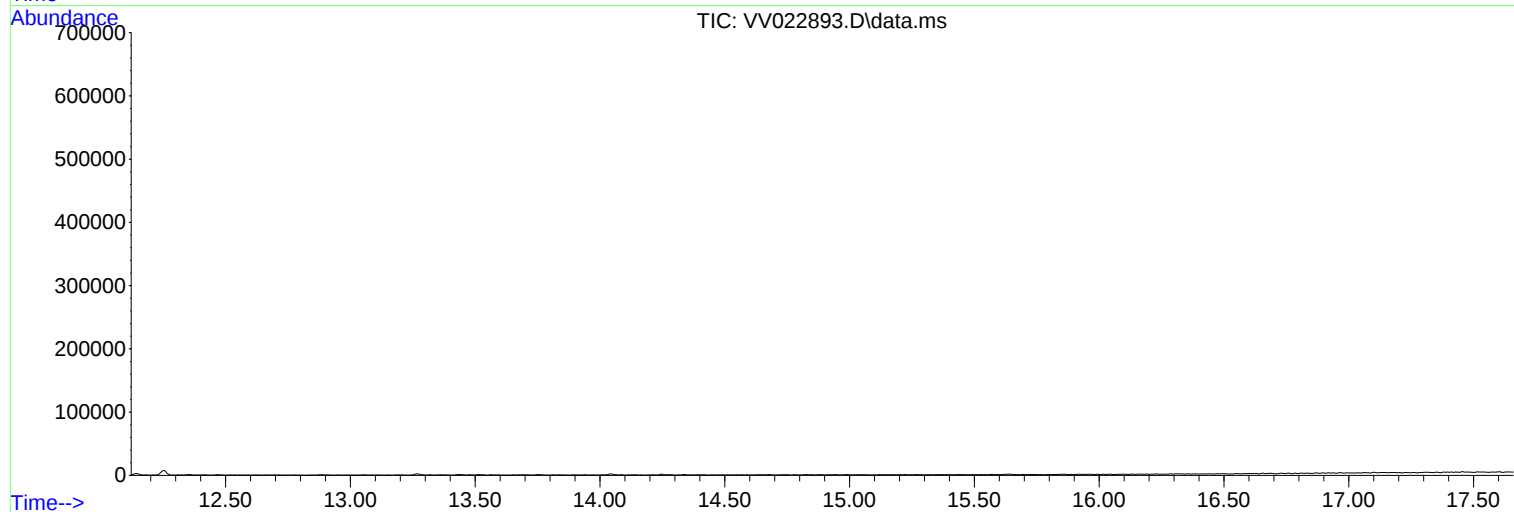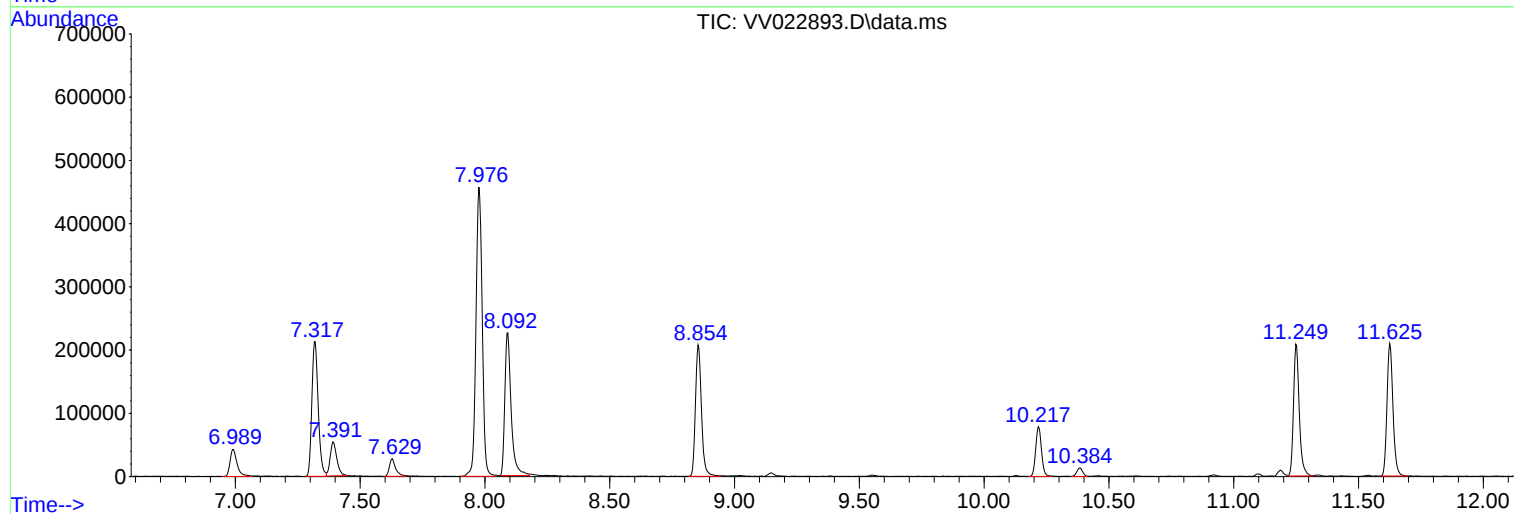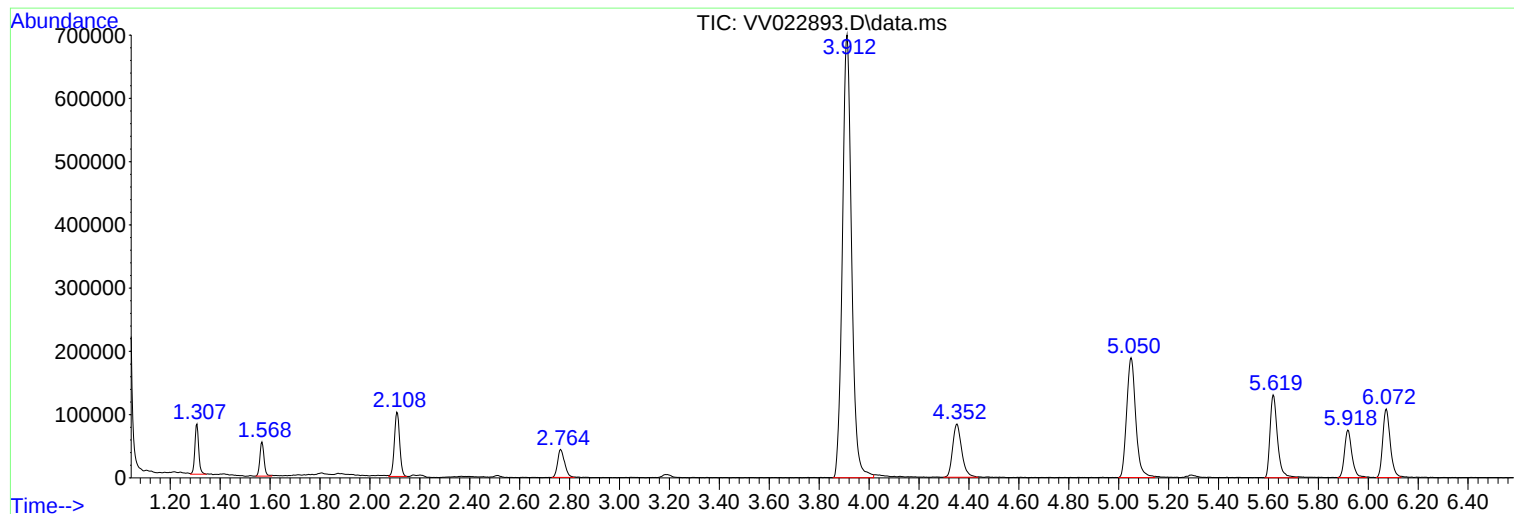

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022893.D
Acq On : 19 Oct 2021 02:17
Operator : SY/MD
Sample : M4137-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022893.D
Acq On : 19 Oct 2021 02:17
Operator : SY/MD
Sample : M4137-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
