

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
 Data File : VV022894.D
 Acq On : 19 Oct 2021 02:41
 Operator : SY/MD
 Sample : M4137-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGBO

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022894.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	94	rVB2	64599	67573	4.21%	0.947%
2	1.568	157	164	179	rVB	51607	56290	3.51%	0.789%
3	2.108	323	332	347	rVB	89138	132244	8.25%	1.854%
4	2.767	525	537	552	rBV3	29142	59795	3.73%	0.838%
5	3.912	876	893	924	rBV2	428905	1151043	71.78%	16.133%
6	4.352	1013	1030	1059	rBV2	86882	226174	14.11%	3.170%
7	5.050	1230	1247	1274	rBV4	189717	484958	30.24%	6.797%
8	5.619	1413	1424	1447	rBV	137472	281867	17.58%	3.951%
9	5.915	1500	1516	1534	rBV	215415	427986	26.69%	5.999%
10	6.072	1551	1565	1592	rBV	114022	236244	14.73%	3.311%
11	6.989	1840	1850	1870	rBV2	45368	86267	5.38%	1.209%
12	7.320	1941	1953	1966	rBV	217269	380217	23.71%	5.329%
13	7.391	1966	1975	1999	rVB	101330	185029	11.54%	2.593%
14	7.625	2037	2048	2063	rBV	28015	50270	3.14%	0.705%
15	7.976	2136	2157	2177	rBV	954814	1603466	100.00%	22.474%
16	8.088	2183	2192	2213	rBV	269917	468598	29.22%	6.568%
17	8.854	2419	2430	2454	rBV	215706	362113	22.58%	5.075%
18	10.217	2843	2854	2871	rBV	88364	140727	8.78%	1.972%
19	10.384	2897	2906	2916	rVB2	13802	21783	1.36%	0.305%
20	11.249	3165	3175	3197	rVV	211338	343739	21.44%	4.818%
21	11.625	3278	3292	3310	rBV	229993	368240	22.97%	5.161%




Sum of corrected areas: 7134623

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022894.D
Acq On : 19 Oct 2021 02:41
Operator : SY/MD
Sample : M4137-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGBO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

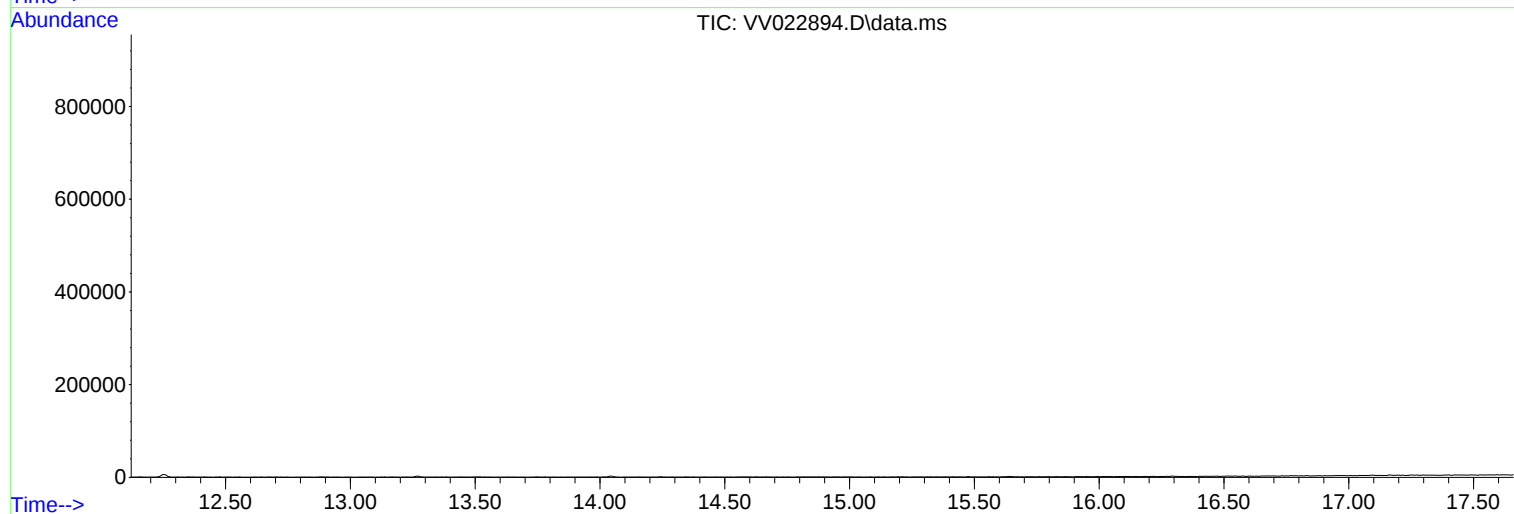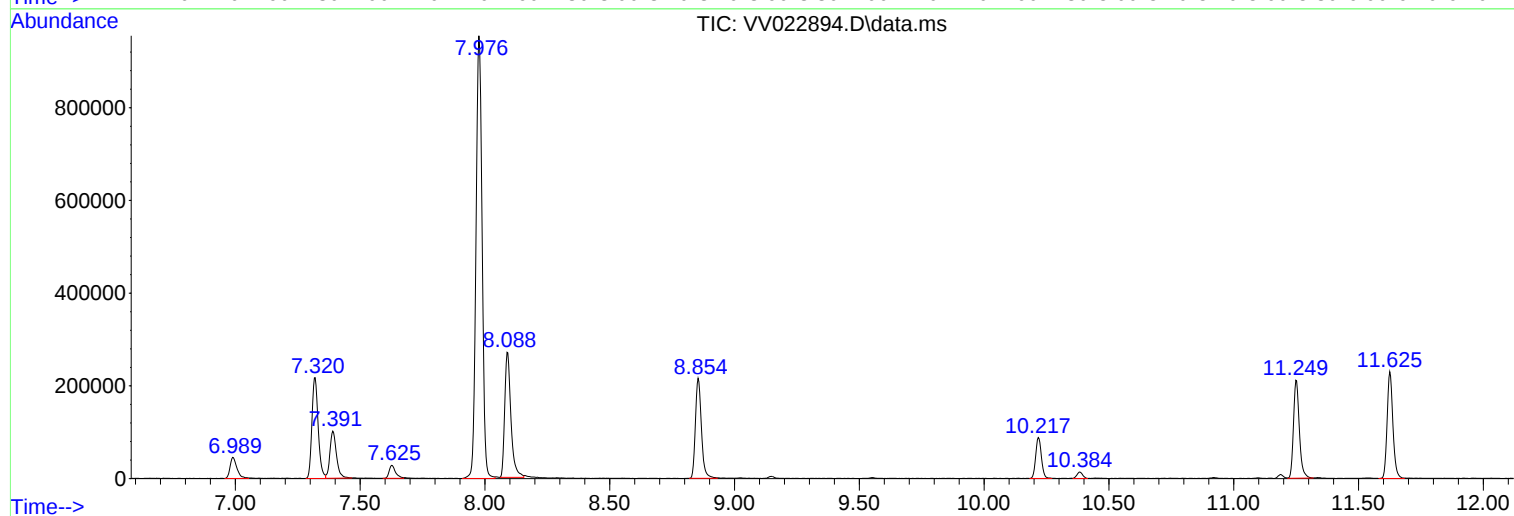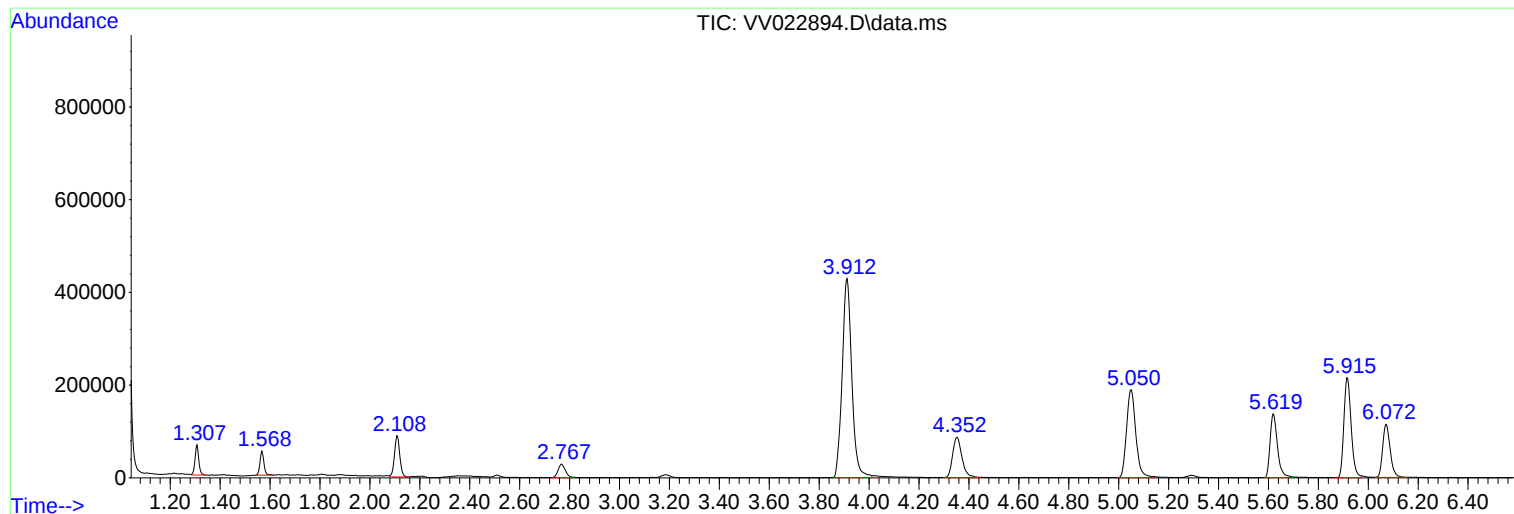

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022894.D
Acq On : 19 Oct 2021 02:41
Operator : SY/MD
Sample : M4137-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022894.D
Acq On : 19 Oct 2021 02:41
Operator : SY/MD
Sample : M4137-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGBO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
