

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
 Data File : VV022897.D
 Acq On : 19 Oct 2021 03:53
 Operator : SY/MD
 Sample : M4137-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGD0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022897.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rVB	53906	56290	8.49%	1.212%
2	1.568	157	164	179	rVB	54587	62234	9.39%	1.340%
3	2.108	319	332	345	rVB	91309	133150	20.09%	2.866%
4	2.365	381	412	455	rBV2	87166	662883	100.00%	14.270%
5	3.886	875	885	923	rBV2	64482	220048	33.20%	4.737%
6	4.352	1013	1030	1055	rBV2	88225	223893	33.78%	4.820%
7	5.050	1230	1247	1281	rBV2	194195	496980	74.97%	10.699%
8	5.619	1412	1424	1449	rBV	136914	282685	42.64%	6.085%
9	6.072	1549	1565	1593	rBV	118593	248384	37.47%	5.347%
10	6.989	1839	1850	1870	rBV2	47366	88353	13.33%	1.902%
11	7.317	1940	1952	1969	rBV	225828	393848	59.41%	8.478%
12	7.394	1969	1976	1987	rVB2	9200	18328	2.76%	0.395%
13	7.625	2039	2048	2068	rBV	27540	50776	7.66%	1.093%
14	8.092	2180	2193	2220	rBV	267072	483549	72.95%	10.409%
15	8.854	2418	2430	2457	rBV	222525	366500	55.29%	7.890%
16	9.146	2512	2521	2531	rBV3	4349	6964	1.05%	0.150%
17	10.217	2843	2854	2871	rBV	91627	147215	22.21%	3.169%
18	10.384	2898	2906	2916	rVB3	4291	6888	1.04%	0.148%
19	11.252	3165	3176	3191	rBV	213219	333818	50.36%	7.186%
20	11.625	3279	3292	3307	rBV	230338	362515	54.69%	7.804%




Sum of corrected areas: 4645301

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022897.D
Acq On : 19 Oct 2021 03:53
Operator : SY/MD
Sample : M4137-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGD0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

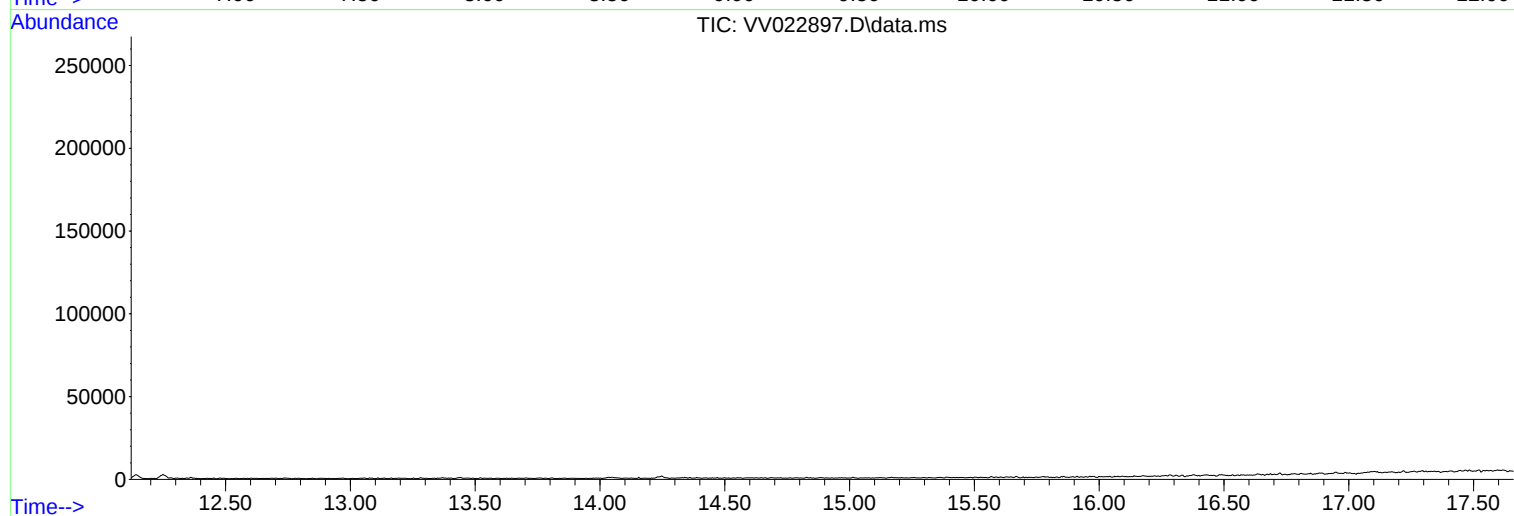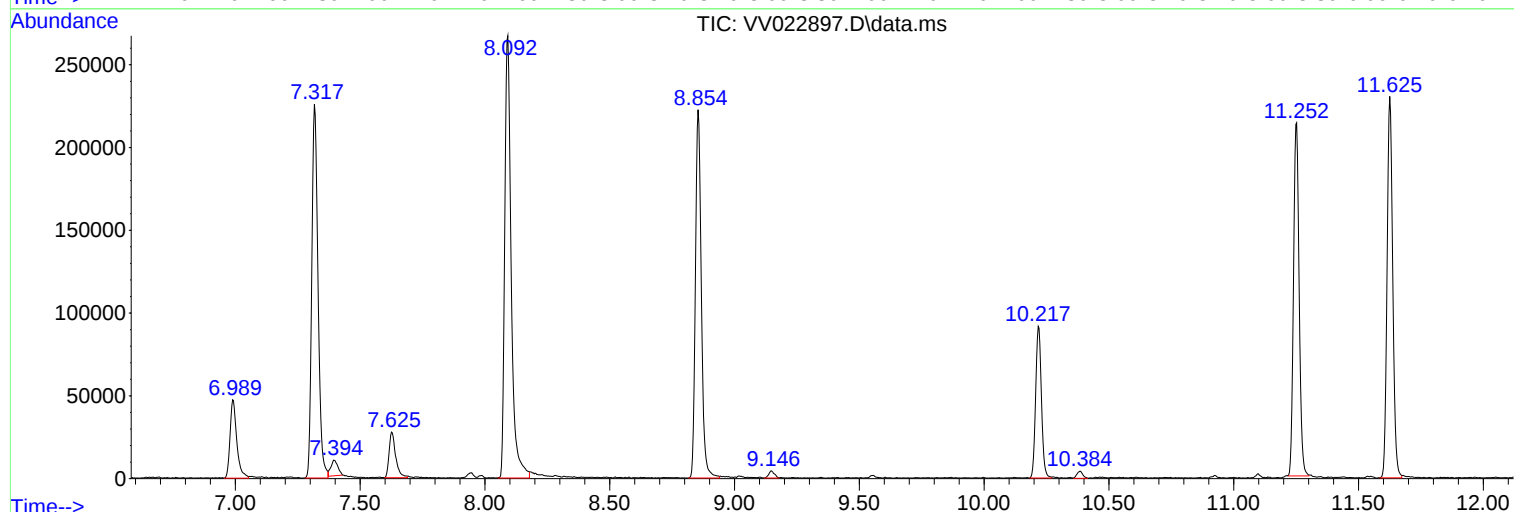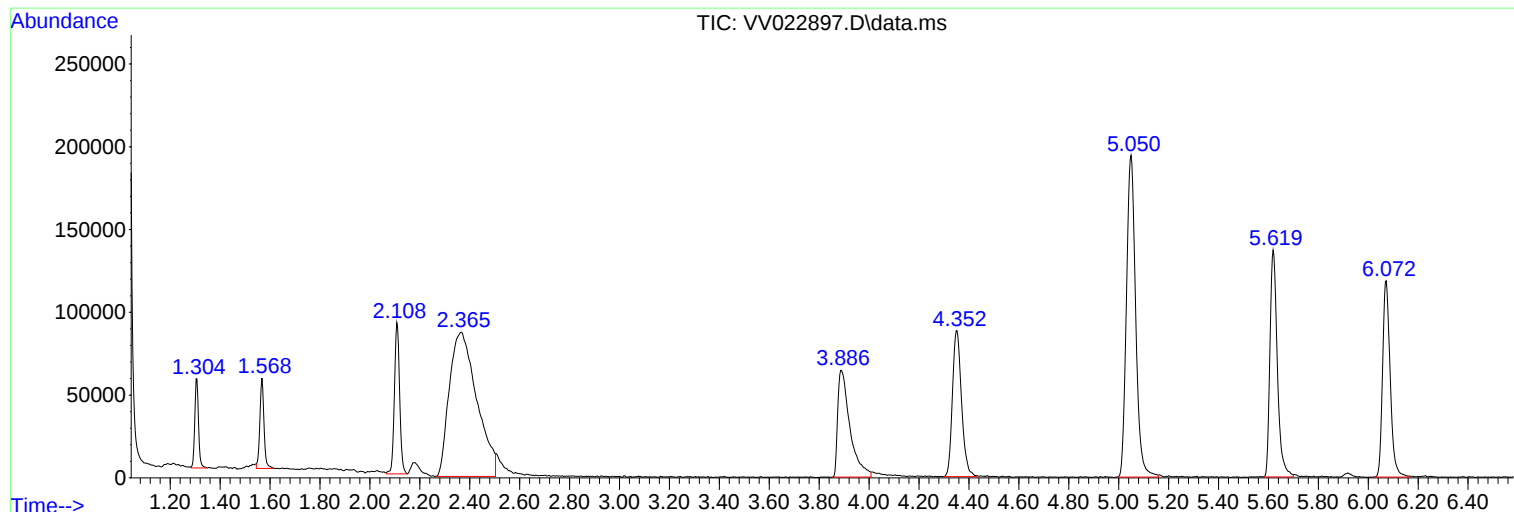

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022897.D
Acq On : 19 Oct 2021 03:53
Operator : SY/MD
Sample : M4137-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGD0










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.365	11.72 ug/L	662883	1,4-Difluorobenzene	5.619

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	83
2			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
3			Isopropyl Alcohol	60	C3H8O	000067-63-0	64
4			Isopropyl Alcohol	60	C3H8O	000067-63-0	64
5			Hydrazine, ethyl-	60	C2H8N2	000624-80-6	40

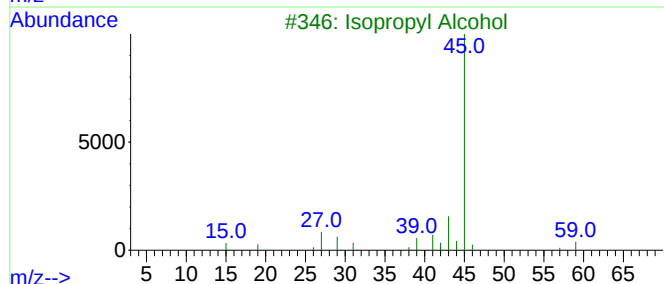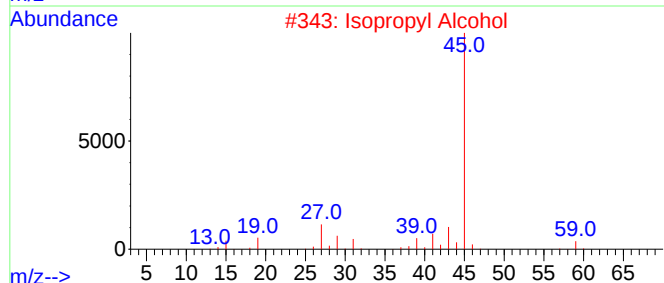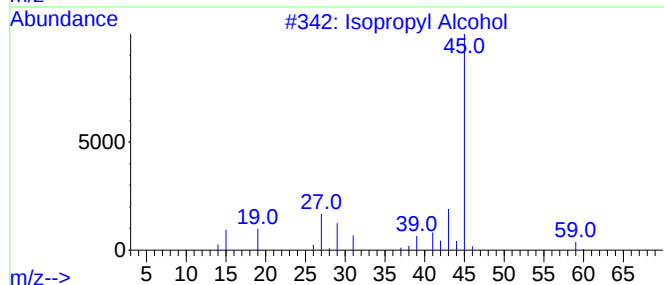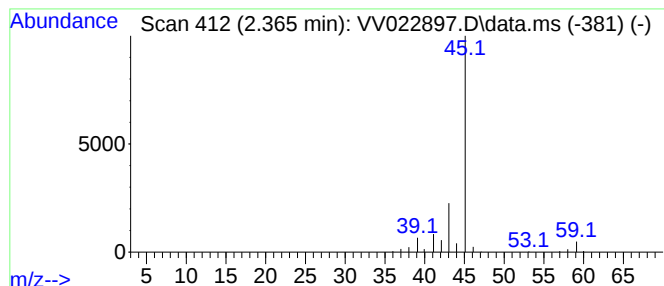

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022897.D
Acq On : 19 Oct 2021 03:53
Operator : SY/MD
Sample : M4137-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGD0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.365	11.7	ug/L	662883	1	5.619	282685	5.0