

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
 Data File : VV022898.D
 Acq On : 19 Oct 2021 04:17
 Operator : SY/MD
 Sample : M4137-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGD1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022898.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	92	rVB	54007	56466	11.85%	1.301%
2	1.568	157	164	177	rVB	53151	59914	12.57%	1.381%
3	2.108	322	332	345	rVB	91833	133779	28.08%	3.083%
4	2.178	345	354	372	rVB2	5370	13531	2.84%	0.312%
5	2.352	383	408	410	rBV2	17023	48862	10.26%	1.126%
6	2.770	523	538	555	rBV2	14856	31142	6.54%	0.718%
7	3.191	657	669	687	rBV3	15137	32437	6.81%	0.748%
8	3.908	876	892	924	rBV3	114188	390681	82.00%	9.003%
9	4.352	1014	1030	1059	rBV2	87785	226019	47.44%	5.209%
10	5.050	1228	1247	1273	rBV2	186768	476454	100.00%	10.980%
11	5.619	1412	1424	1452	rBV	134813	277915	58.33%	6.404%
12	5.921	1506	1518	1536	rBV5	14460	31841	6.68%	0.734%
13	6.069	1550	1564	1589	rBV2	111406	234971	49.32%	5.415%
14	6.989	1840	1850	1874	rBV	44177	83826	17.59%	1.932%
15	7.316	1940	1952	1969	rBV	211507	374632	78.63%	8.633%
16	7.397	1970	1977	1990	rVB	11066	21336	4.48%	0.492%
17	7.625	2039	2048	2062	rBV3	26765	48203	10.12%	1.111%
18	7.979	2137	2158	2171	rBV	68999	121380	25.48%	2.797%
19	8.088	2183	2192	2228	rBV	264718	474681	99.63%	10.939%
20	8.853	2419	2430	2454	rBV	214719	359552	75.46%	8.286%
21	9.146	2511	2521	2537	rVB2	6336	11992	2.52%	0.276%
22	10.217	2843	2854	2867	rBV	88942	139241	29.22%	3.209%
23	10.384	2892	2906	2915	rBV5	3282	5330	1.12%	0.123%
24	11.098	3119	3128	3135	rBV4	4076	6404	1.34%	0.148%
25	11.249	3162	3175	3191	rBV	211736	325623	68.34%	7.504%
26	11.625	3280	3292	3306	rBV	222931	353166	74.12%	8.139%




Sum of corrected areas: 4339378

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022898.D
Acq On : 19 Oct 2021 04:17
Operator : SY/MD
Sample : M4137-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGD1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

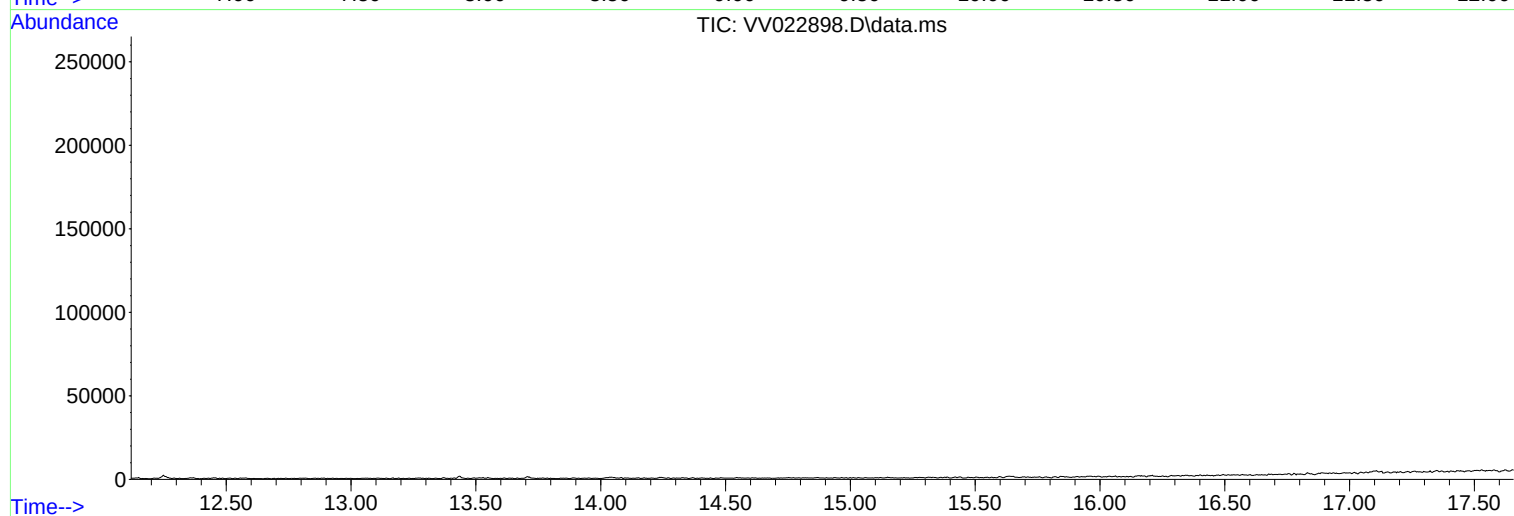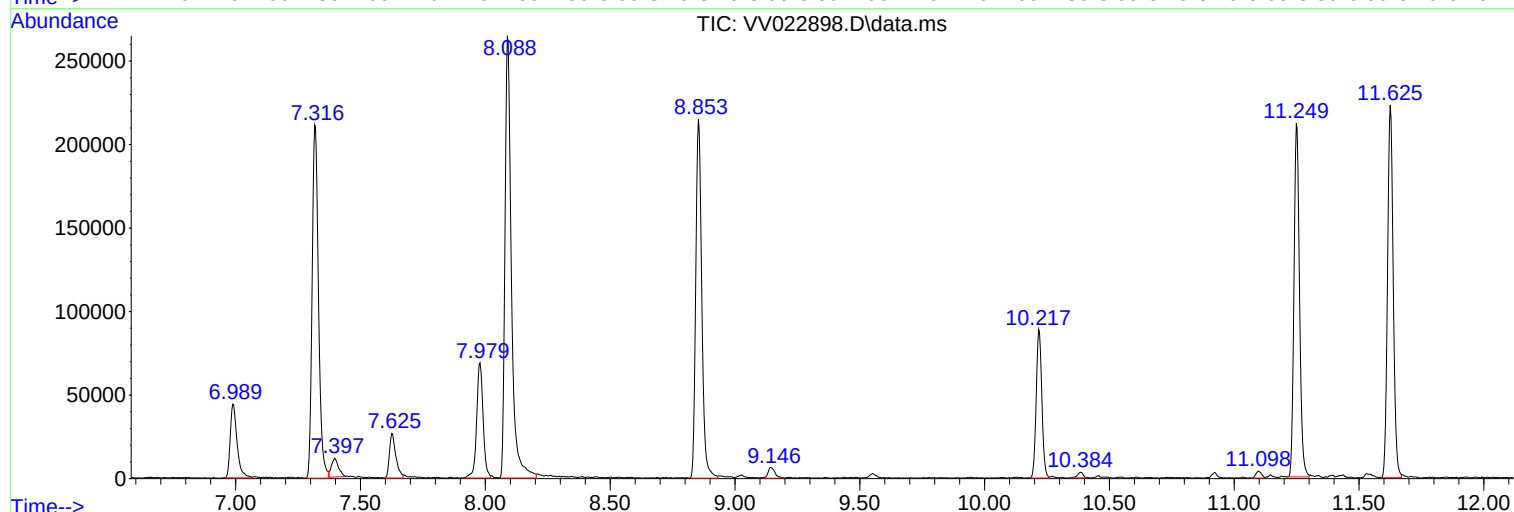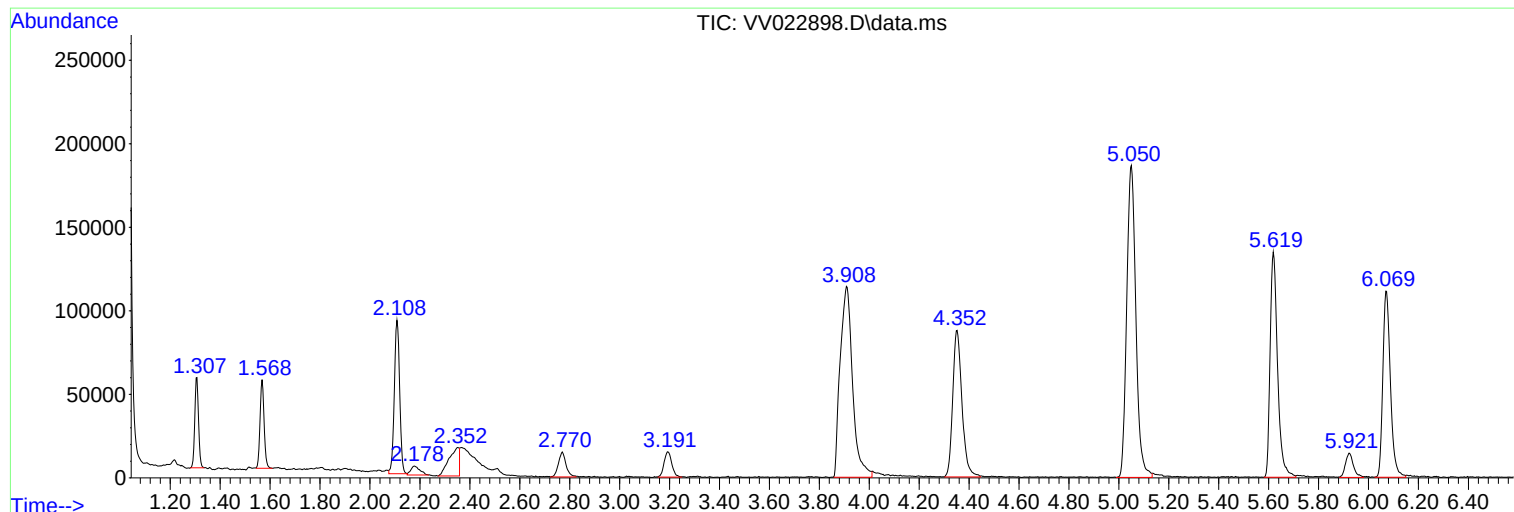

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022898.D
Acq On : 19 Oct 2021 04:17
Operator : SY/MD
Sample : M4137-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGD1










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.352	0.88 ug/L	48862	1,4-Difluorobenzene	5.619

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	56
2			Isopropyl Alcohol	60	C3H8O	000067-63-0	9
3			Isopropyl Alcohol	60	C3H8O	000067-63-0	9
4			Ethylamine	45	C2H7N	000075-04-7	7
5			2-Propanone, 1-methoxy-	88	C4H8O2	005878-19-3	4

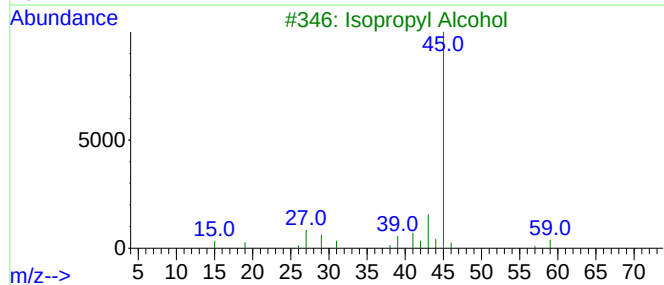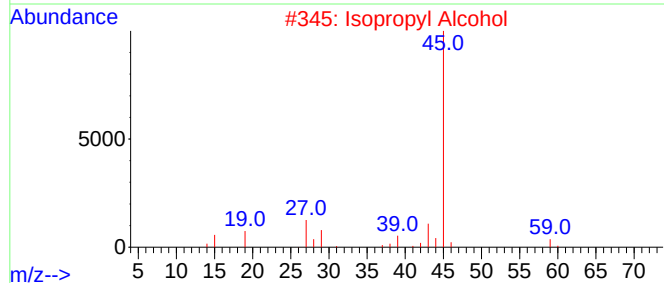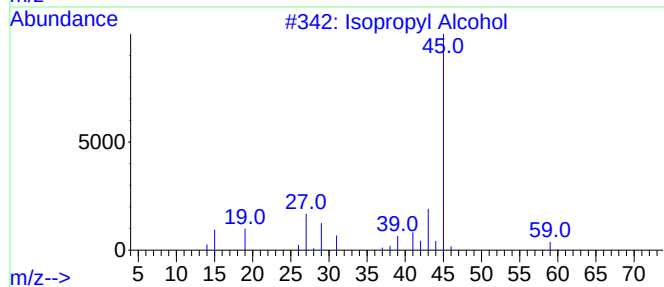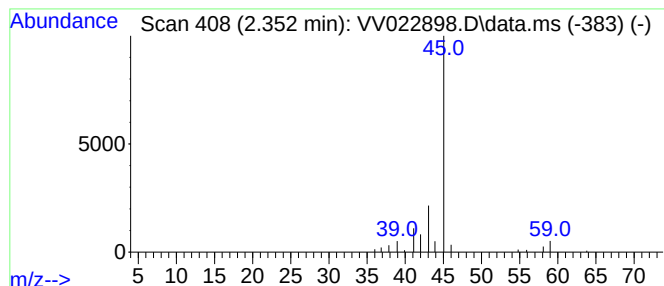

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022898.D
Acq On : 19 Oct 2021 04:17
Operator : SY/MD
Sample : M4137-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGD1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.352	0.9	ug/L	48862	1	5.619	277915	5.0