

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
 Data File : VV022903.D
 Acq On : 19 Oct 2021 06:17
 Operator : SY/MD
 Sample : M4137-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGD6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022903.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	95	rVB	53488	55005	11.91%	1.442%
2	1.568	156	164	174	rBV	49528	56648	12.26%	1.485%
3	1.806	233	238	246	rVB3	6603	8247	1.79%	0.216%
4	2.108	322	332	343	rBV	89196	129653	28.07%	3.399%
5	2.179	343	354	377	rVB	24258	58966	12.77%	1.546%
6	2.349	384	407	409	rBV9	9815	26826	5.81%	0.703%
7	3.886	875	885	919	rBV2	52233	166483	36.04%	4.365%
8	4.352	1014	1030	1054	rBV2	83033	210498	45.57%	5.519%
9	5.050	1231	1247	1279	rBV2	182162	461884	100.00%	12.110%
10	5.619	1413	1424	1448	rBV	139202	285679	61.85%	7.490%
11	6.072	1552	1565	1595	rBV	108208	228479	49.47%	5.991%
12	6.989	1840	1850	1867	rBV	43001	78188	16.93%	2.050%
13	7.317	1937	1952	1970	rBV	205756	367209	79.50%	9.628%
14	7.397	1970	1977	1995	rVB2	9813	21323	4.62%	0.559%
15	7.625	2037	2048	2065	rBV	25603	46430	10.05%	1.217%
16	7.944	2137	2147	2153	rBV3	3187	5154	1.12%	0.135%
17	8.091	2183	2193	2216	rBV	223234	403147	87.28%	10.570%
18	8.854	2418	2430	2455	rBV	218423	366084	79.26%	9.599%
19	9.146	2513	2521	2528	rBV4	4636	7192	1.56%	0.189%
20	9.870	2735	2746	2752	rBV6	5064	7876	1.71%	0.207%
21	10.217	2843	2854	2872	rBV2	80155	128913	27.91%	3.380%
22	10.384	2894	2906	2916	rVB2	4717	7337	1.59%	0.192%
23	11.098	3119	3128	3135	rBV3	5262	8395	1.82%	0.220%
24	11.249	3165	3175	3191	rBV	216353	332981	72.09%	8.731%
25	11.625	3281	3292	3310	rBV	212808	339756	73.56%	8.908%
26	12.252	3476	3487	3493	rBV6	3328	5580	1.21%	0.146%




Sum of corrected areas: 3813933

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022903.D
Acq On : 19 Oct 2021 06:17
Operator : SY/MD
Sample : M4137-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGD6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

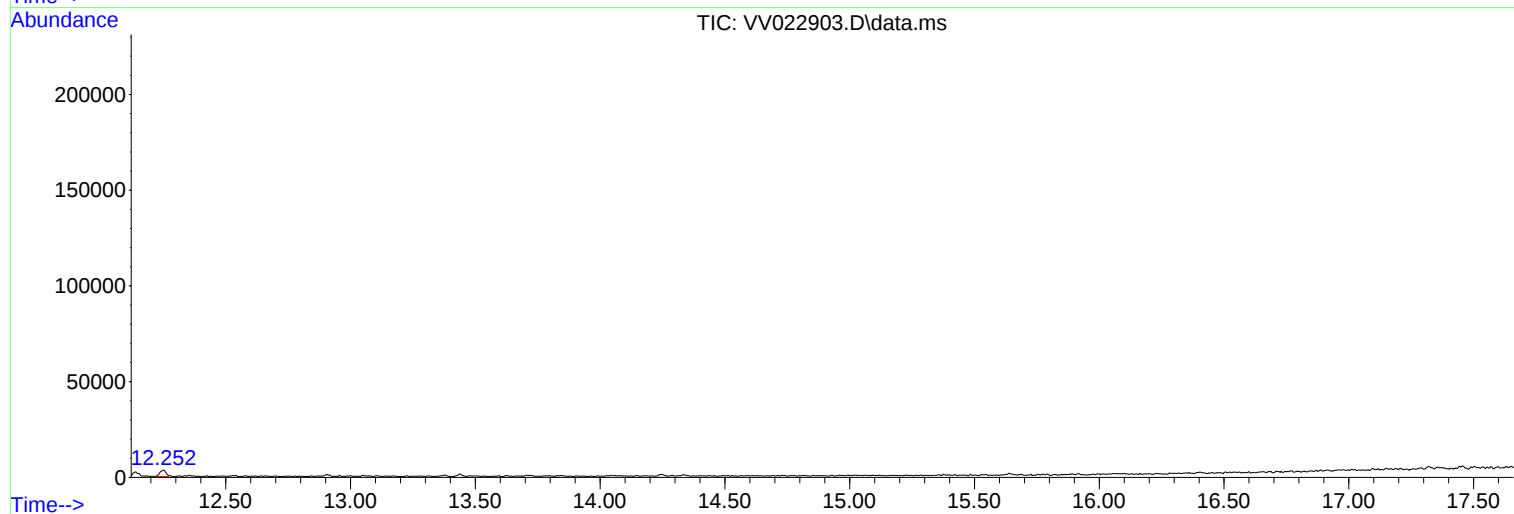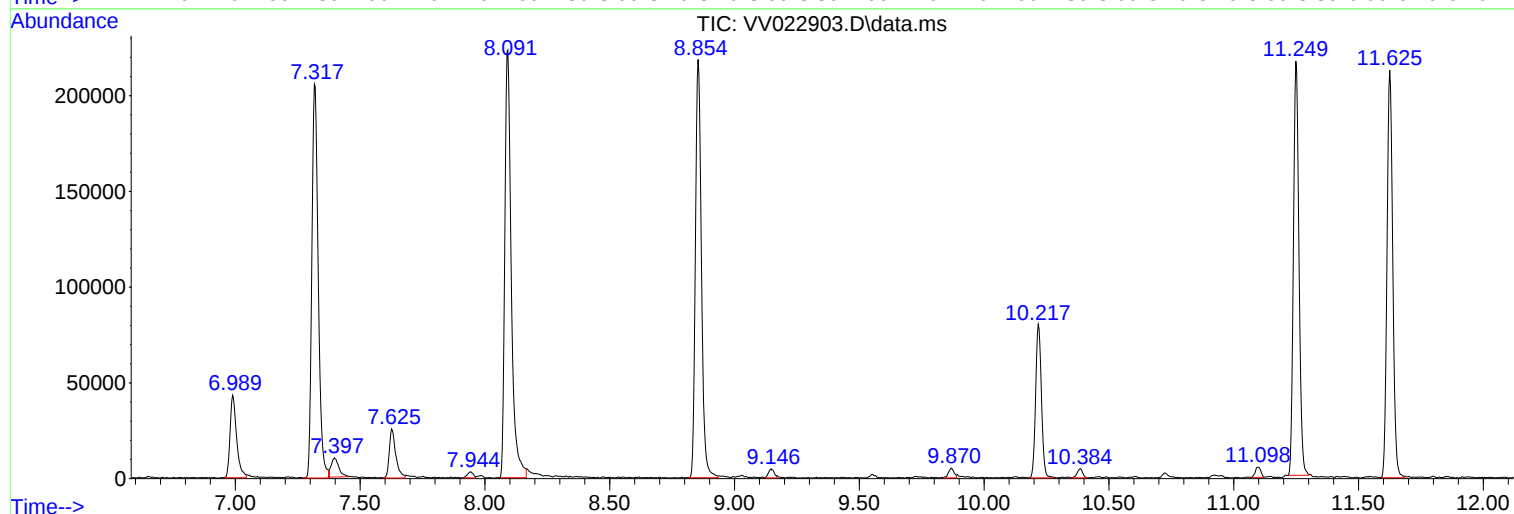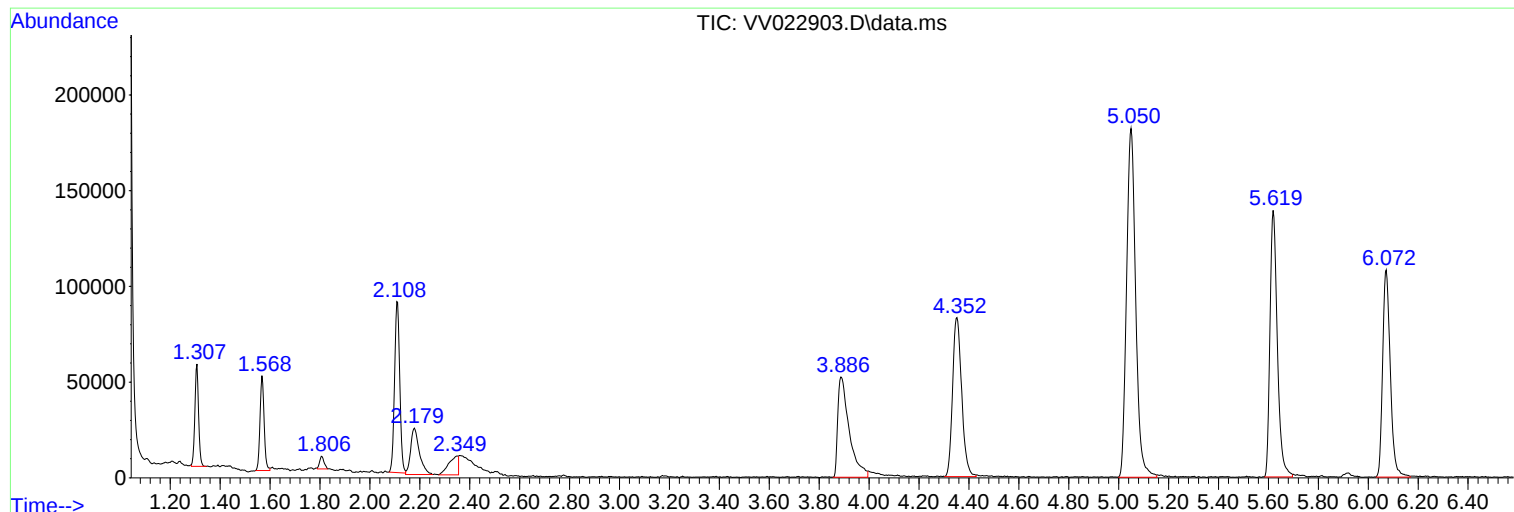

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022903.D
Acq On : 19 Oct 2021 06:17
Operator : SY/MD
Sample : M4137-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGD6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
Data File : VV022903.D
Acq On : 19 Oct 2021 06:17
Operator : SY/MD
Sample : M4137-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGD6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
