
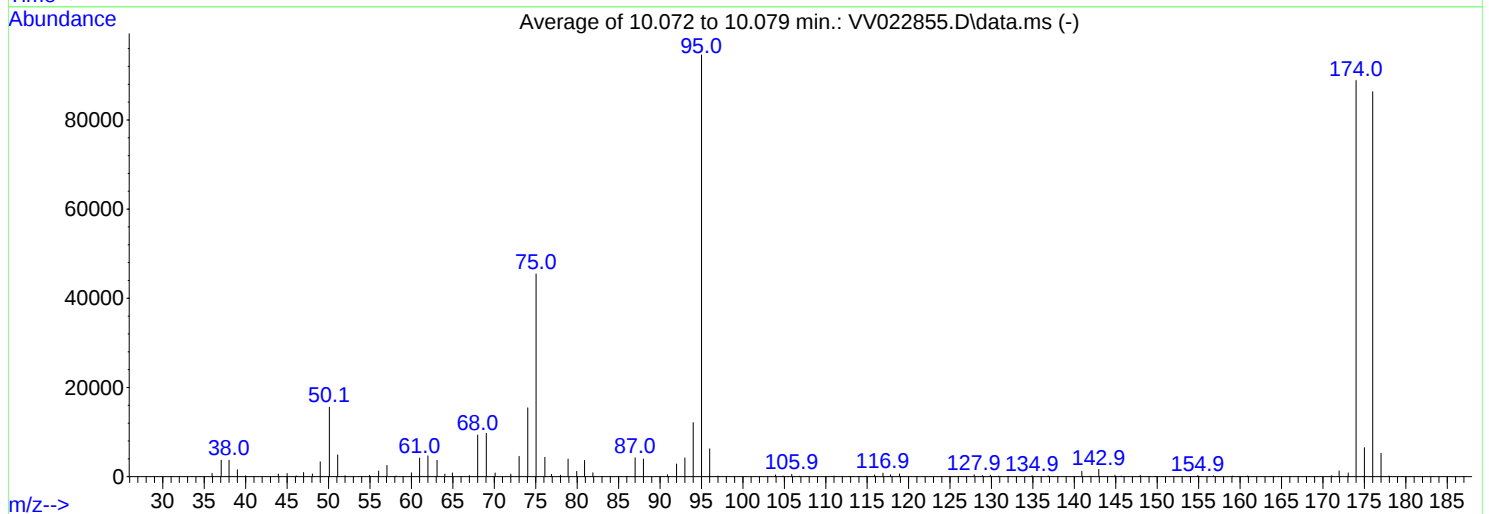


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101821\
 Data File : VV022855.D
 Acq On : 18 Oct 2021 09:20
 Operator : SY/MD
 Sample : BFB217
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB217

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue Oct 19 04:07:06 2021

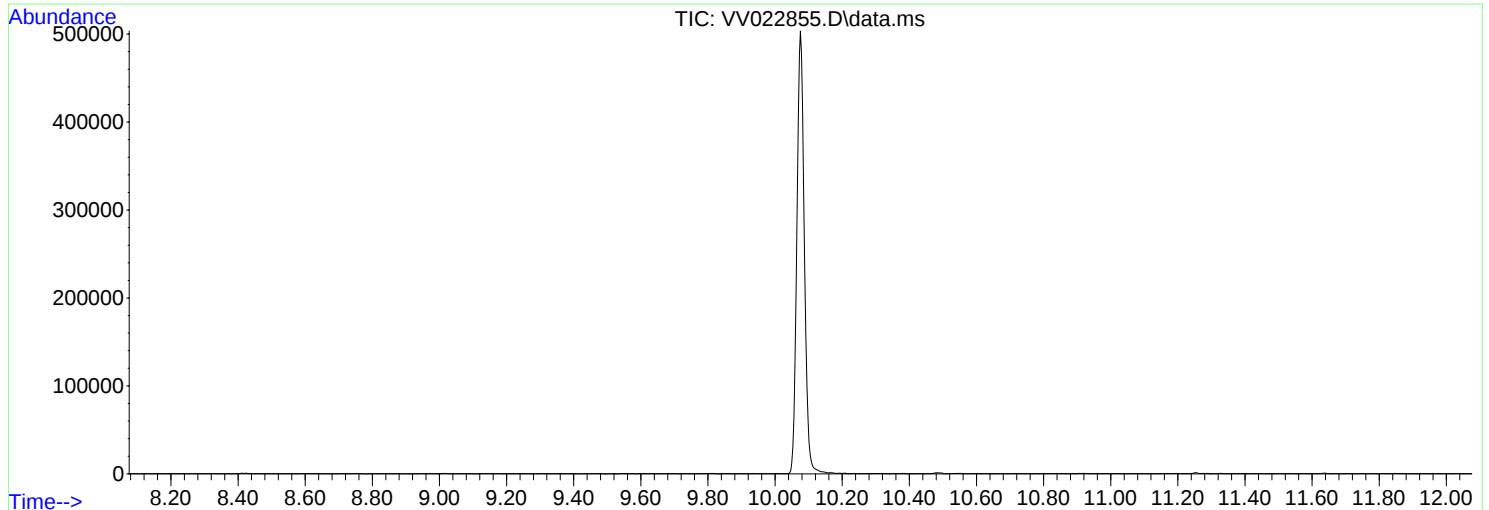

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	15569	PASS
75	95	30	80	48.1	45469	PASS
95	95	100	100	100.0	94597	PASS
96	95	5	9	6.6	6263	PASS
173	174	0.00	2	0.9	815	PASS
174	95	50	120	93.9	88859	PASS
175	174	5	9	7.3	6514	PASS
176	174	95	105	97.1	86323	PASS
177	176	5	10	6.1	5249	PASS

m/z	Abundance
43.90	151.0

Instrument :
MSVOA_V
ClientSampleId :
BFB217

m/z	Abundance
36.00	772.0
37.00	3562.0
38.00	3797.0
39.00	1448.0
40.00	259.0
44.00	735.0
45.00	686.0
46.10	211.0
47.00	907.0
48.00	634.0
49.00	3370.0
50.10	15685.0
51.10	4796.0
52.00	213.0
54.90	305.0
56.00	1198.0
57.00	2453.0
58.20	111.0
60.00	844.0
61.00	4004.0
62.00	4643.0
63.10	3794.0
64.10	574.0
64.90	794.0
67.00	207.0
68.00	9141.0
69.10	9788.0
70.10	781.0
72.00	485.0
73.00	4585.0
74.00	15451.0
75.10	45504.0
76.10	4306.0
76.90	508.0
78.00	281.0
78.90	3891.0
79.90	1150.0
80.90	3629.0
81.90	867.0
83.00	147.0
85.90	152.0
86.10	155.0
87.00	4064.0
88.00	3975.0
90.90	505.0
92.00	2914.0
93.00	4252.0
94.00	11983.0
95.00	93216.0
96.00	6523.0
97.00	124.0
103.90	393.0
104.90	183.0
105.90	461.0
106.90	130.0
111.00	142.0
114.90	138.0
115.90	392.0
116.90	752.0
117.80	431.0
118.90	552.0
127.90	416.0
128.90	241.0
129.80	388.0
130.80	154.0
134.90	221.0
136.90	188.0
140.90	1082.0
141.90	173.0
143.00	1519.0
144.90	351.0
145.60	138.0
147.90	279.0
153.90	116.0
154.90	278.0
156.80	239.0
159.10	116.0
160.90	136.0
171.00	176.0
171.90	1277.0
173.00	1211.0
174.00	85192.0
175.00	6420.0
176.00	82992.0
177.00	5189.0
178.00	134.0

Instrument :
MSVOA_V
ClientSampleId :
BFB217

m/z	Abundance
36.00	748.0
37.00	3766.0
38.00	3835.0
39.00	1579.0
40.00	240.0
44.00	780.0
45.00	732.0
46.10	179.0
47.00	956.0
48.00	651.0
49.00	3457.0
50.10	16061.0
51.10	5063.0
52.00	203.0
54.90	298.0
56.00	1295.0
57.10	2605.0
58.10	138.0
60.00	873.0
61.00	4261.0
62.00	4876.0
63.10	3813.0
64.10	598.0
65.00	892.0
67.00	266.0
68.00	9742.0
69.10	10015.0
70.10	861.0
72.00	597.0
73.00	4732.0
74.10	15978.0
75.00	46952.0
76.10	4510.0
76.90	527.0
78.00	331.0
78.90	4110.0
80.00	1236.0
80.90	3794.0
81.90	855.0
83.00	113.0
87.00	4462.0
88.00	4121.0
90.90	449.0
92.00	2922.0
93.00	4295.0
94.00	12586.0
95.00	98160.0
96.00	6522.0
97.00	136.0
103.90	413.0
104.80	162.0
105.90	560.0
106.80	135.0
110.00	126.0
111.00	170.0
112.80	103.0
114.90	125.0
115.90	411.0
116.90	788.0
117.80	464.0
118.90	644.0
127.90	444.0
128.90	252.0
129.90	342.0
130.80	138.0
134.90	257.0
136.90	175.0
140.90	1242.0
141.90	151.0
143.00	1688.0
144.90	342.0
145.70	150.0
148.00	316.0
149.80	116.0
154.90	272.0
156.80	240.0
159.00	166.0
160.90	163.0
171.10	222.0
172.00	1340.0
173.10	1233.0
174.00	92192.0
175.00	6762.0
176.00	89496.0
177.00	5383.0
177.90	161.0

Instrument :
MSVOA_V
ClientSampleId :
BFB217

m/z	Abundance
35.90	738.0
37.10	3718.0
38.00	3497.0
39.00	1619.0
40.00	184.0
44.00	706.0
45.00	772.0
46.10	103.0
47.00	977.0
48.10	609.0
49.00	3184.0
50.10	14961.0
51.10	4785.0
52.00	197.0
55.00	263.0
56.10	1231.0
57.10	2458.0
58.10	144.0
60.00	869.0
61.00	4198.0
62.00	4496.0
63.10	3373.0
64.00	532.0
65.00	838.0
67.00	301.0
68.00	9143.0
69.00	9402.0
70.10	836.0
72.00	686.0
73.00	4327.0
74.10	14897.0
75.00	43952.0
76.10	4225.0
76.90	528.0
78.00	342.0
78.90	3818.0
80.00	1137.0
80.90	3465.0
81.90	858.0
87.00	4145.0
88.00	3725.0
90.90	394.0
92.00	2661.0
93.00	4103.0
94.00	11816.0
95.00	92416.0
96.00	5743.0
97.00	150.0
104.00	412.0
104.80	136.0
105.90	552.0
106.80	107.0
109.90	143.0
111.00	159.0
112.80	124.0
114.90	119.0
115.90	432.0
116.90	798.0
117.80	442.0
118.90	666.0
123.90	113.0
127.90	415.0
128.90	268.0
129.90	344.0
130.90	128.0
134.90	244.0
136.80	151.0
140.90	1288.0
142.90	1639.0
144.90	323.0
145.70	142.0
147.90	294.0
149.80	108.0
154.90	286.0
156.80	212.0
159.00	183.0
160.90	186.0
171.10	207.0
172.00	1293.0
174.00	89192.0
175.00	6360.0
176.00	86480.0
177.00	5176.0
178.00	187.0

Instrument :
MSVOA_V
ClientSampleId :
BFB217