

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101822\
 Data File : VV028603.D
 Acq On : 18 Oct 2022 10:20
 Operator : SY/MD
 Sample : VV1018WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK252

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028603.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	74	81	92	rVB	116495	116399	17.10%	2.058%
2	1.561	154	162	179	rVB	110082	129000	18.95%	2.281%
3	2.098	320	329	345	rVB	188480	270199	39.69%	4.778%
4	2.500	443	454	464	rBV4	11142	20375	2.99%	0.360%
5	3.905	880	891	910	rBV2	47469	162945	23.94%	2.882%
6	4.336	1008	1025	1046	rBV	113131	288465	42.37%	5.101%
7	5.037	1226	1243	1267	rBV2	270990	680778	100.00%	12.039%
8	5.606	1408	1420	1446	rBV	227684	474556	69.71%	8.392%
9	6.063	1547	1562	1583	rBV	159455	345590	50.76%	6.112%
10	6.982	1837	1848	1866	rBV	71617	140962	20.71%	2.493%
11	7.307	1936	1949	1974	rBV	299745	546275	80.24%	9.661%
12	7.619	2038	2046	2064	rBV2	37416	73391	10.78%	1.298%
13	8.085	2181	2191	2226	rBV	279245	620294	91.12%	10.970%
14	8.844	2415	2427	2447	rBV	342482	577142	84.78%	10.207%
15	10.207	2841	2851	2865	rBV	100090	161131	23.67%	2.850%
16	11.239	3161	3172	3196	rBV	332605	547985	80.49%	9.691%
17	11.615	3277	3289	3310	rBV	270056	444863	65.35%	7.867%
18	13.259	3793	3800	3808	rVB	6176	8554	1.26%	0.151%
19	13.503	3865	3876	3888	rBV3	8504	17299	2.54%	0.306%
20	13.741	3939	3950	3958	rBV3	6755	11278	1.66%	0.199%
21	15.879	4603	4615	4618	rVV3	8045	17124	2.52%	0.303%




Sum of corrected areas: 5654605

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101822\
Data File : VV028603.D
Acq On : 18 Oct 2022 10:20
Operator : SY/MD
Sample : VV1018WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK252

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

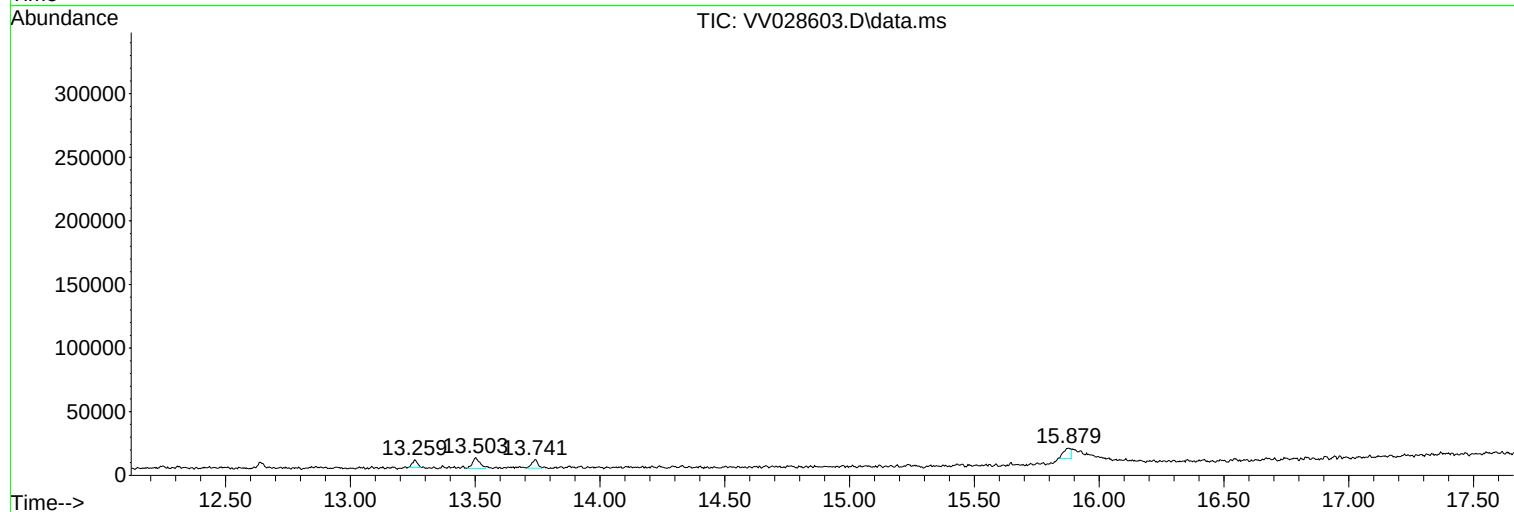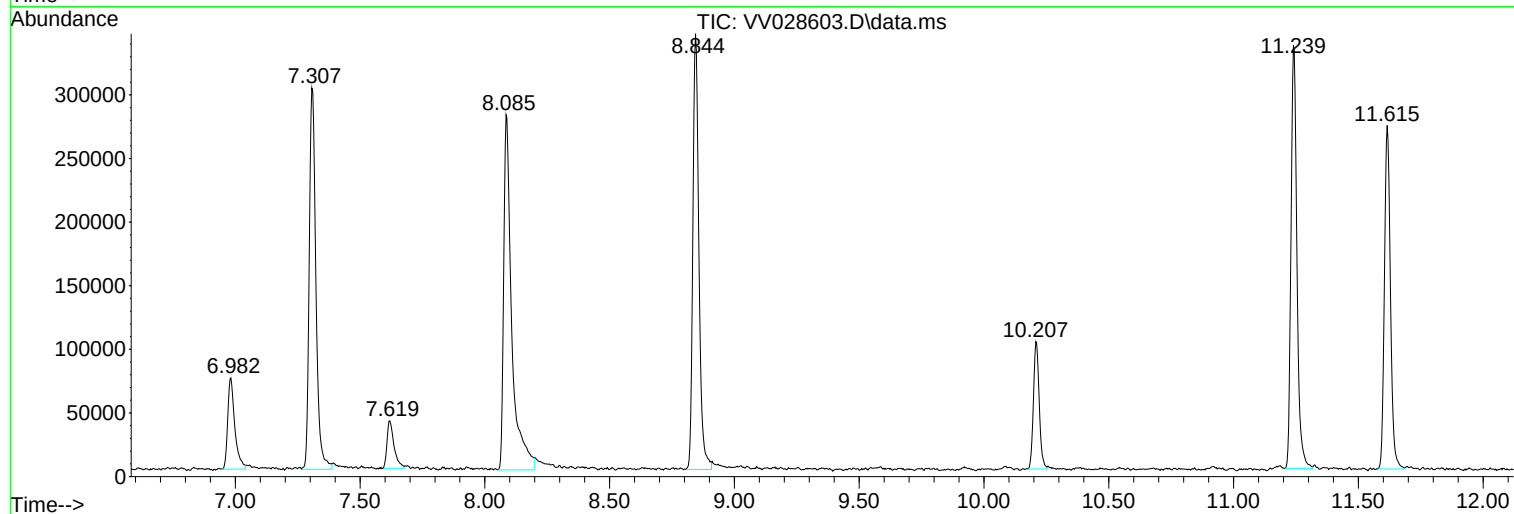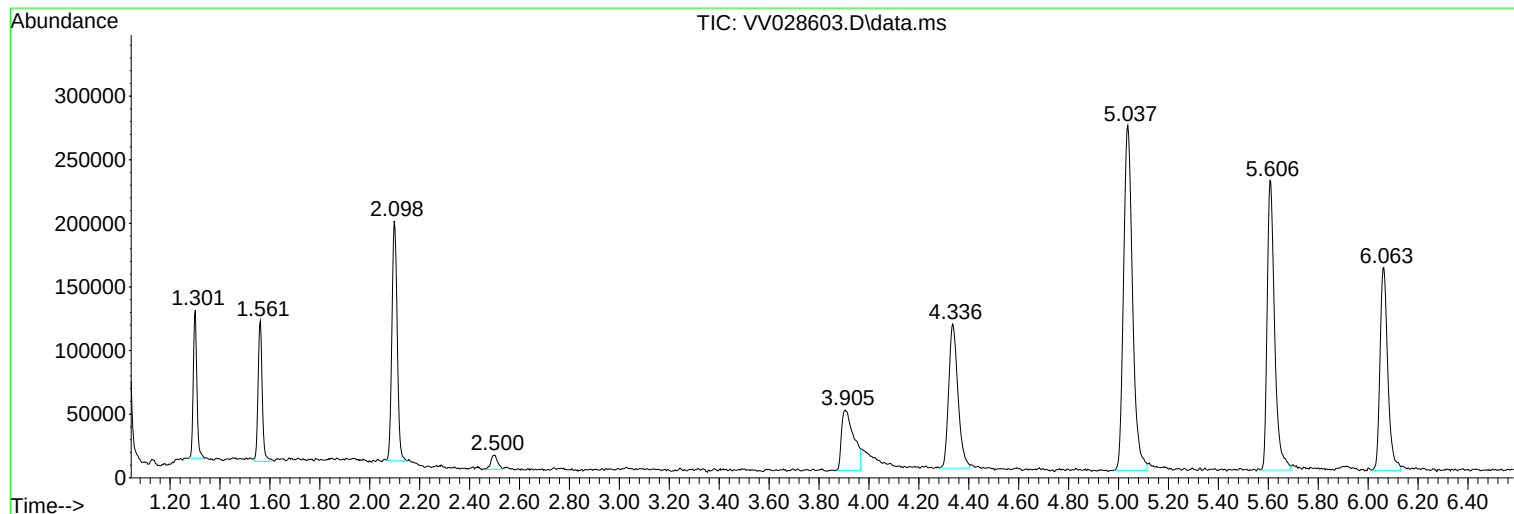

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101822\
Data File : VV028603.D
Acq On : 18 Oct 2022 10:20
Operator : SY/MD
Sample : VV1018WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK252

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101822\
Data File : VV028603.D
Acq On : 18 Oct 2022 10:20
Operator : SY/MD
Sample : VV1018WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK252

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------