

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101822\
 Data File : VV028605.D
 Acq On : 18 Oct 2022 11:11
 Operator : SY/MD
 Sample : N5163-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BD719

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028605.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.233	51	60	64	rBV2	10954	19193	2.20%	0.291%
2	1.294	73	79	92	rVB	112843	116491	13.33%	1.765%
3	1.558	154	161	172	rVB	111660	123928	14.18%	1.877%
4	2.095	319	328	339	rBV	185910	262359	30.02%	3.975%
5	3.950	890	905	930	rBV2	68868	286849	32.83%	4.346%
6	4.336	1012	1025	1042	rVB	148165	353959	40.51%	5.362%
7	5.031	1227	1241	1265	rBV2	386696	873832	100.00%	13.238%
8	5.603	1407	1419	1440	rBV	281850	553376	63.33%	8.384%
9	6.056	1549	1560	1575	rBV	216250	423415	48.45%	6.415%
10	6.976	1832	1846	1862	rBV	75120	133728	15.30%	2.026%
11	7.301	1936	1947	1961	rBV	305294	522254	59.77%	7.912%
12	7.375	1961	1970	1983	rVB	137822	232003	26.55%	3.515%
13	7.616	2036	2045	2064	rVB2	40298	71795	8.22%	1.088%
14	7.931	2135	2143	2156	rVB2	10089	20960	2.40%	0.318%
15	8.104	2185	2197	2237	rBV	312690	656294	75.11%	9.943%
16	8.844	2415	2427	2452	rBV	314970	528665	60.50%	8.009%
17	9.005	2468	2477	2489	rBV	18903	33460	3.83%	0.507%
18	9.130	2506	2516	2532	rBV	70189	118902	13.61%	1.801%
19	9.539	2633	2643	2655	rBV	32602	56894	6.51%	0.862%
20	10.211	2837	2852	2871	rBV	104208	172734	19.77%	2.617%
21	10.371	2891	2902	2914	rVB4	24069	44631	5.11%	0.676%
22	10.439	2914	2923	2924	rBV4	10296	10002	1.14%	0.152%
23	10.905	3060	3068	3081	rBV	19208	32378	3.71%	0.491%
24	11.239	3160	3172	3190	rBV	307223	489996	56.07%	7.423%
25	11.529	3254	3262	3270	rBV	9178	15128	1.73%	0.229%
26	11.616	3277	3289	3308	rBV	263736	425235	48.66%	6.442%
27	12.342	3504	3515	3522	rBV	5978	10847	1.24%	0.164%
28	13.500	3864	3875	3882	rBV3	6362	11395	1.30%	0.173%




Sum of corrected areas: 6600703

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101822\
Data File : VV028605.D
Acq On : 18 Oct 2022 11:11
Operator : SY/MD
Sample : N5163-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BD719

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

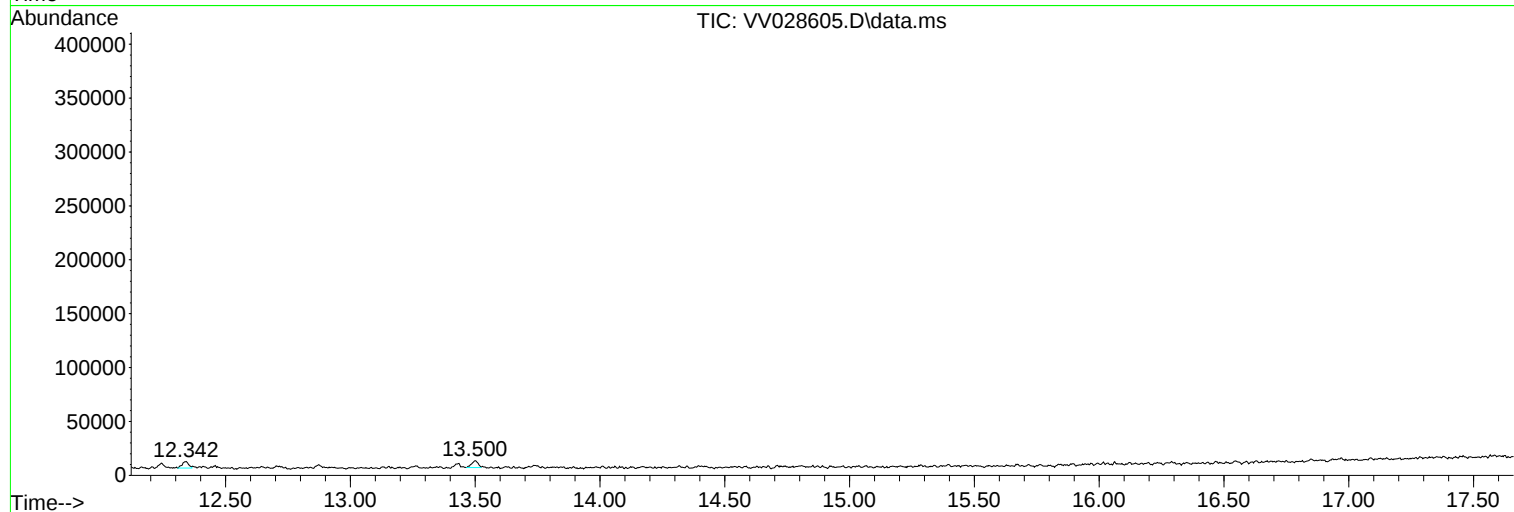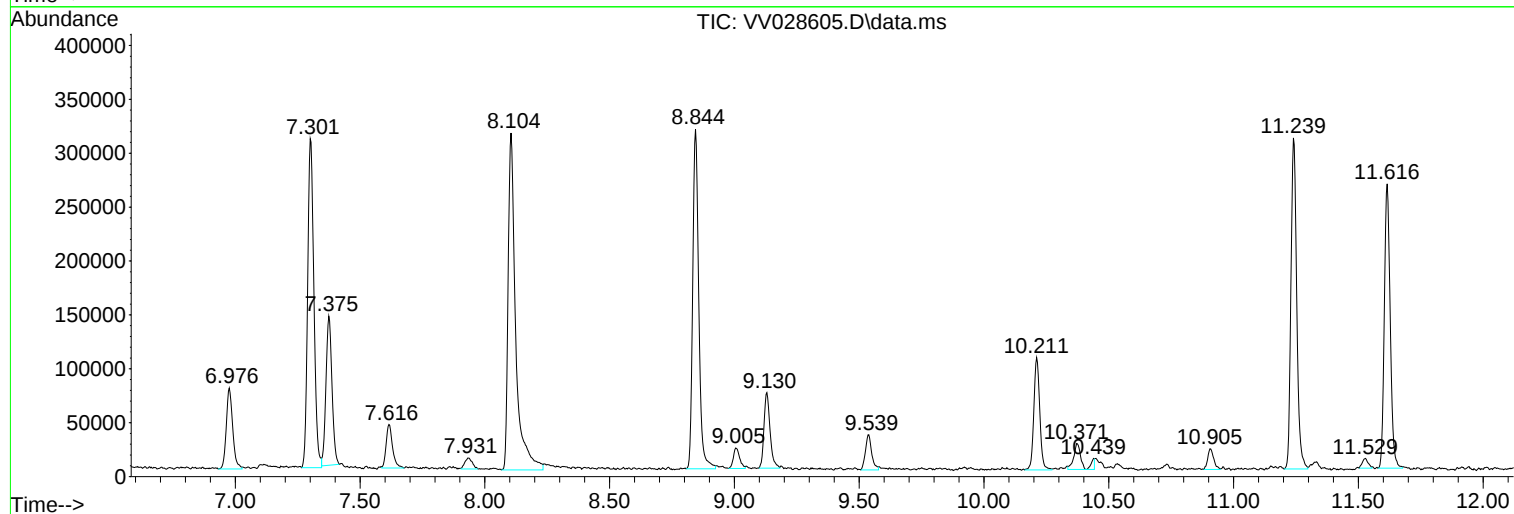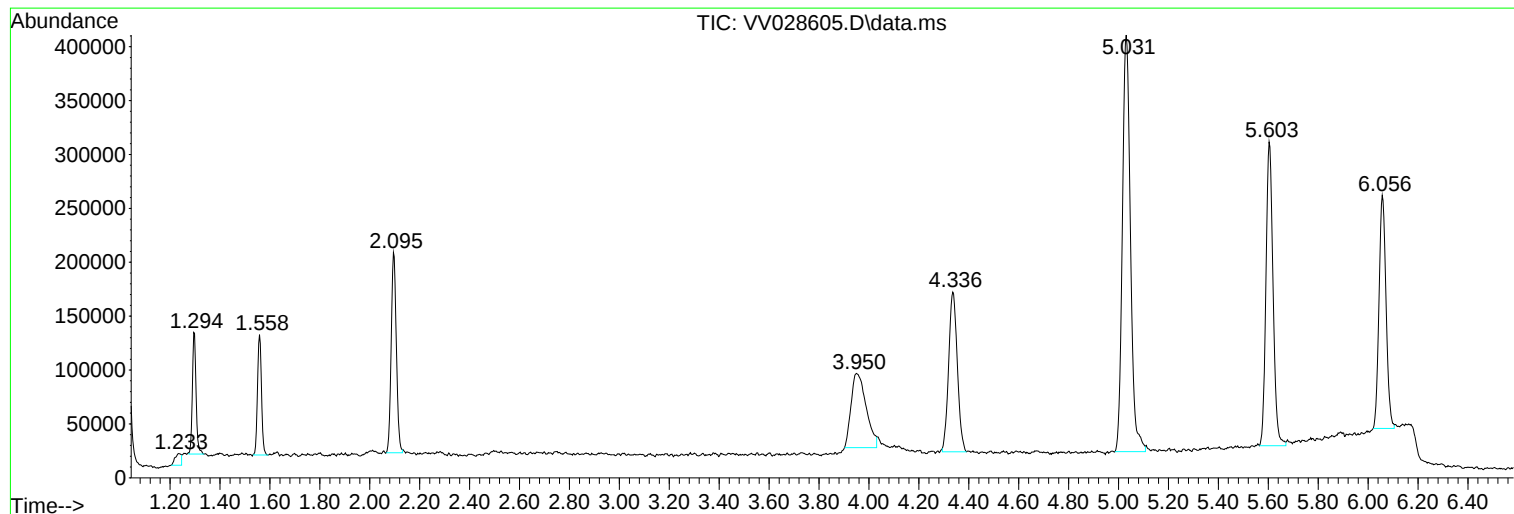

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101822\
Data File : VV028605.D
Acq On : 18 Oct 2022 11:11
Operator : SY/MD
Sample : N5163-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BD719

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101822\
Data File : VV028605.D
Acq On : 18 Oct 2022 11:11
Operator : SY/MD
Sample : N5163-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BD719

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc