

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101822\
 Data File : VV028609.D
 Acq On : 18 Oct 2022 12:44
 Operator : SY/MD
 Sample : N5163-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BD713

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028609.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	95	rVB	97776	101794	3.60%	1.238%
2	1.561	155	162	175	rBV	96000	108042	3.82%	1.314%
3	2.101	319	330	344	rBV	168325	241017	8.52%	2.931%
4	3.902	879	890	918	rBV3	52939	197295	6.98%	2.400%
5	4.342	1012	1027	1048	rBV	105132	266527	9.43%	3.242%
6	5.040	1230	1244	1267	rBV3	251343	633119	22.39%	7.700%
7	5.612	1409	1422	1447	rBV	217646	456279	16.14%	5.549%
8	6.066	1549	1563	1589	rBV	153586	325144	11.50%	3.954%
9	6.985	1838	1849	1867	rBV	64669	130859	4.63%	1.592%
10	7.310	1939	1950	1967	rBV	275434	500586	17.70%	6.088%
11	7.390	1967	1975	1988	rVB2	20275	42294	1.50%	0.514%
12	7.622	2035	2047	2063	rBV3	34598	72321	2.56%	0.880%
13	7.969	2131	2155	2175	rBV	1680006	2827692	100.00%	34.391%
14	8.088	2183	2192	2233	rBV	250776	615684	21.77%	7.488%
15	8.847	2414	2428	2446	rBV	327021	562442	19.89%	6.840%
16	10.210	2840	2852	2870	rBV	98234	165871	5.87%	2.017%
17	10.378	2892	2904	2913	rBV3	17967	31013	1.10%	0.377%
18	11.242	3162	3173	3196	rBV	318226	522096	18.46%	6.350%
19	11.615	3277	3289	3313	rVB	255740	422200	14.93%	5.135%




Sum of corrected areas: 8222275

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101822\
Data File : VV028609.D
Acq On : 18 Oct 2022 12:44
Operator : SY/MD
Sample : N5163-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BD713

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

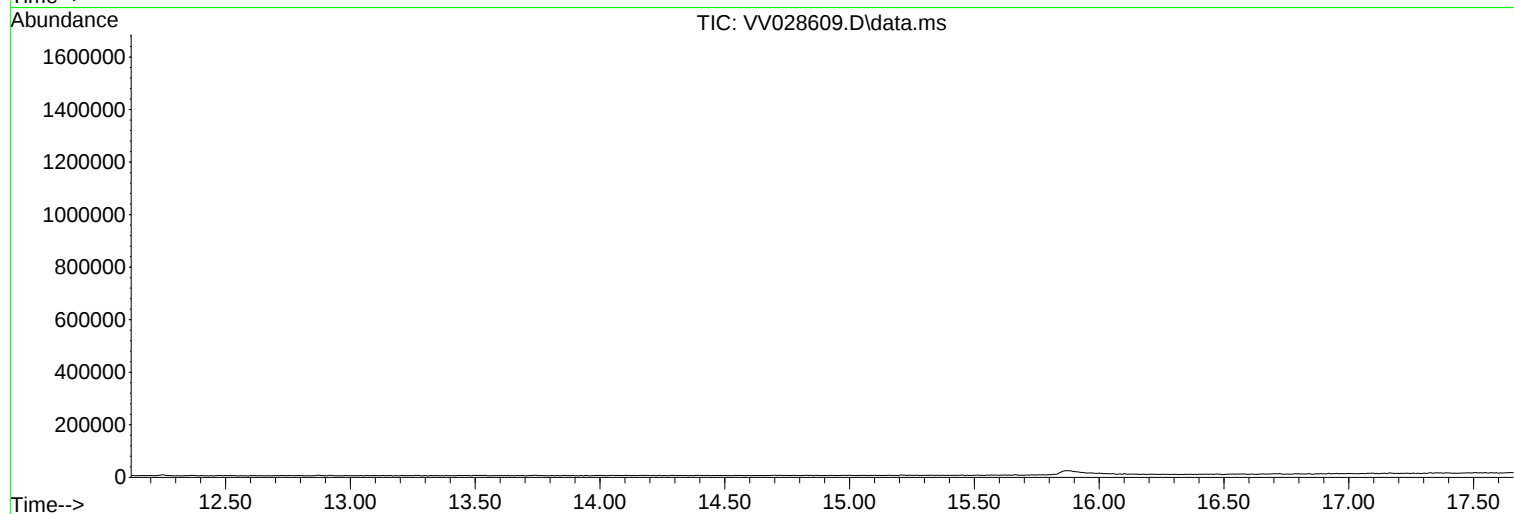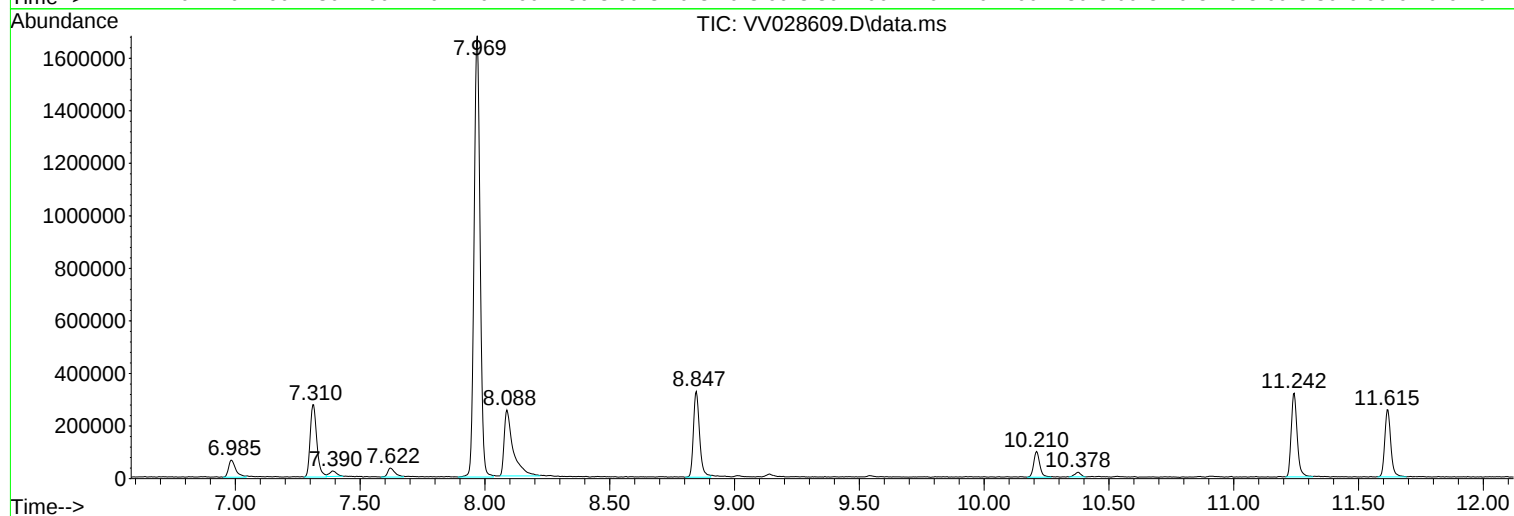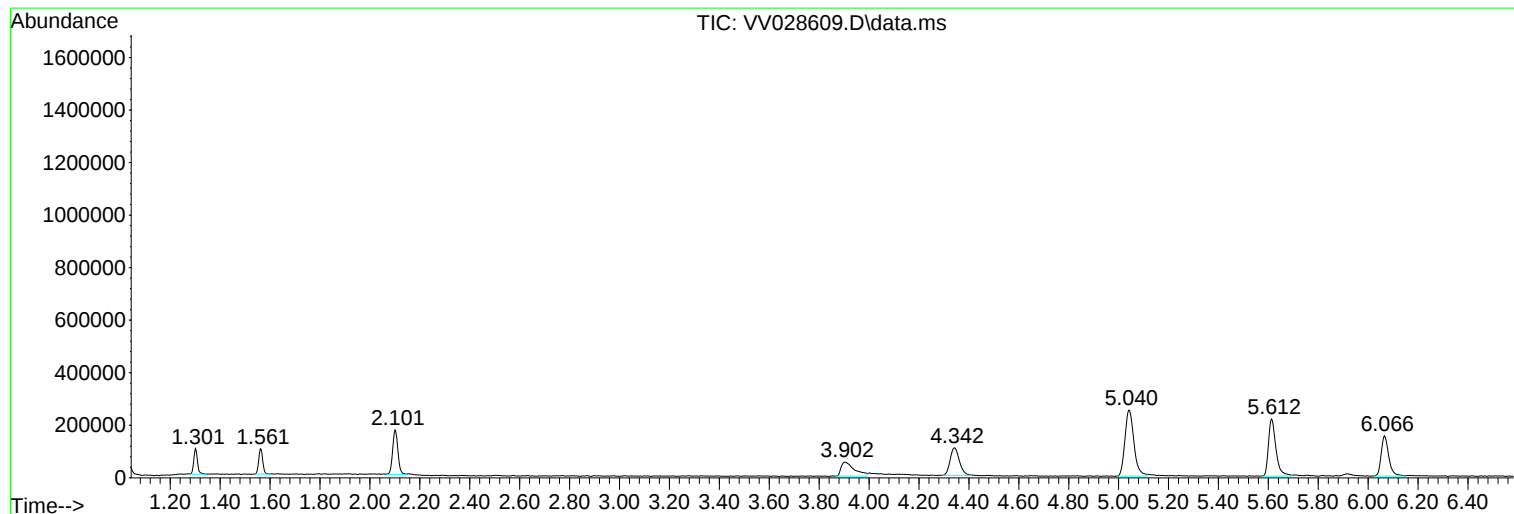

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101822\
Data File : VV028609.D
Acq On : 18 Oct 2022 12:44
Operator : SY/MD
Sample : N5163-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BD713

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101822\
Data File : VV028609.D
Acq On : 18 Oct 2022 12:44
Operator : SY/MD
Sample : N5163-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BD713

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------