

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101822\
 Data File : VV028614.D
 Acq On : 18 Oct 2022 14:43
 Operator : SY/MD
 Sample : N5173-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFXS6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028614.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	55	62	71	rBV3	10522	17843	2.71%	0.336%
2	1.304	75	82	96	rVB	95904	97918	14.88%	1.846%
3	1.564	156	163	178	rVB	98496	112410	17.08%	2.119%
4	2.105	320	331	342	rBV	164574	237635	36.11%	4.480%
5	3.905	882	891	907	rBV2	37020	115680	17.58%	2.181%
6	4.342	1014	1027	1051	rVB	111241	279455	42.46%	5.269%
7	5.043	1228	1245	1270	rBV2	259277	658101	100.00%	12.408%
8	5.612	1411	1422	1442	rBV	207753	433950	65.94%	8.182%
9	6.066	1549	1563	1586	rBV	158697	340043	51.67%	6.411%
10	6.985	1839	1849	1866	rBV	65357	129716	19.71%	2.446%
11	7.313	1939	1951	1970	rBV	283812	511843	77.78%	9.650%
12	7.622	2037	2047	2065	rBV2	35216	70152	10.66%	1.323%
13	7.976	2148	2157	2168	rVB2	10864	20817	3.16%	0.392%
14	8.088	2181	2192	2237	rBV	232461	656618	99.77%	12.380%
15	8.847	2415	2428	2449	rBV	316629	538813	81.87%	10.159%
16	10.210	2842	2852	2867	rBV	99019	164940	25.06%	3.110%
17	11.242	3163	3173	3193	rBV	301214	483674	73.50%	9.119%
18	11.532	3254	3263	3278	rBV	5918	11143	1.69%	0.210%
19	11.615	3278	3289	3311	rBV	259534	423211	64.31%	7.979%




Sum of corrected areas: 5303962

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101822\
Data File : VV028614.D
Acq On : 18 Oct 2022 14:43
Operator : SY/MD
Sample : N5173-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXS6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

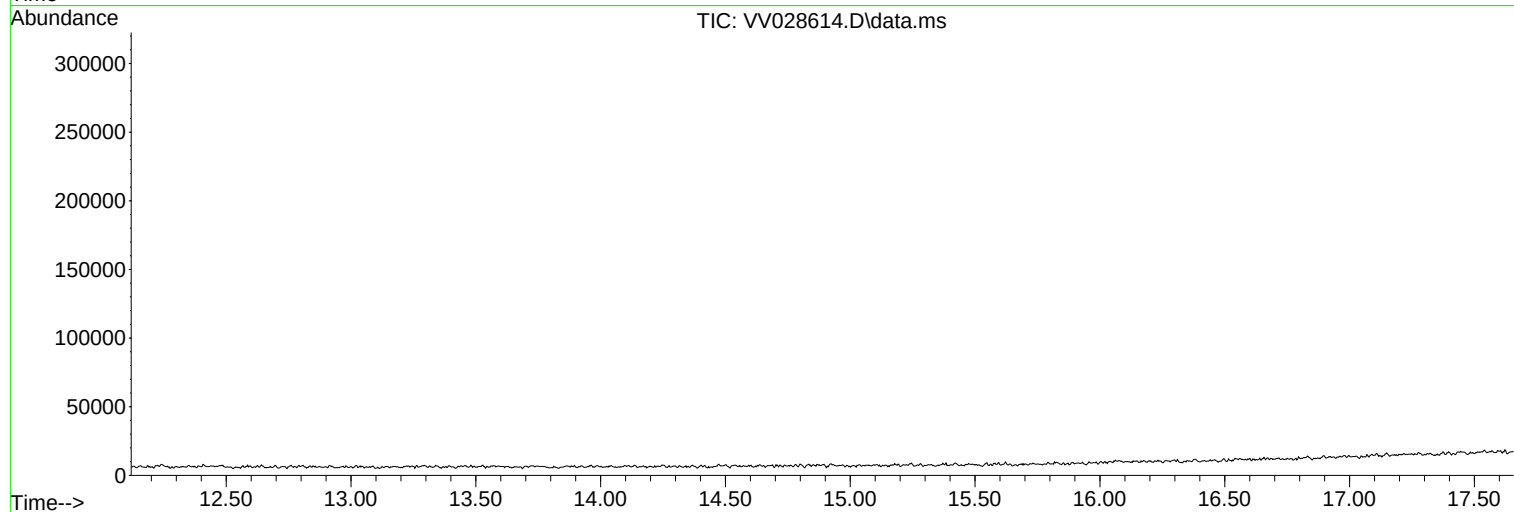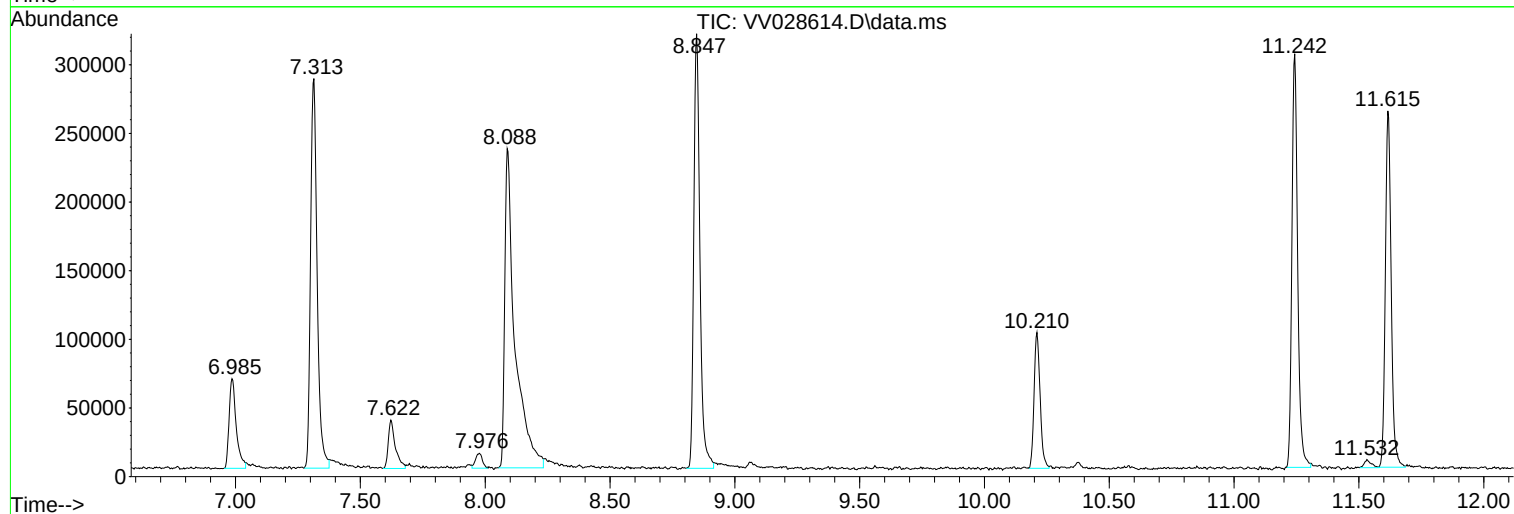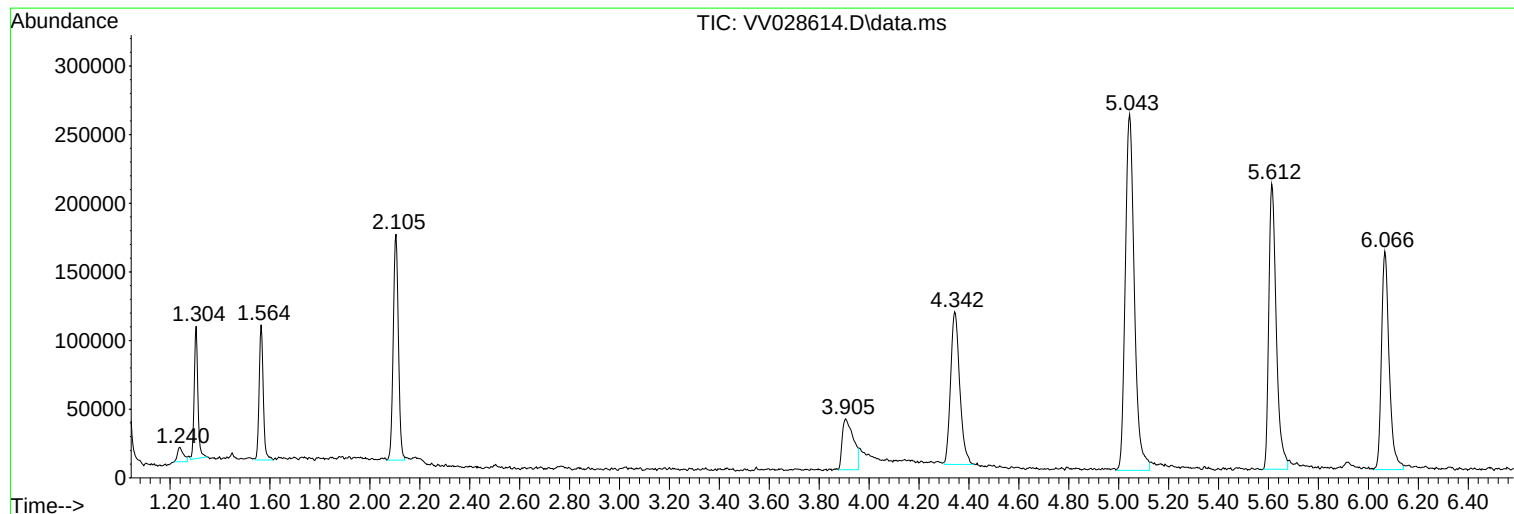

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101822\
Data File : VV028614.D
Acq On : 18 Oct 2022 14:43
Operator : SY/MD
Sample : N5173-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXS6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101822\
Data File : VV028614.D
Acq On : 18 Oct 2022 14:43
Operator : SY/MD
Sample : N5173-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXS6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------