

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101822\
 Data File : VV028615.D
 Acq On : 18 Oct 2022 15:07
 Operator : SY/MD
 Sample : N5173-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFXS7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028615.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.127	21	27	41	rBV2	152343	175214	4.52%	1.385%
2	1.298	74	80	92	rVB	98579	97303	2.51%	0.769%
3	1.558	154	161	172	rVB	100501	110315	2.84%	0.872%
4	2.098	319	329	344	rVB2	167390	249967	6.44%	1.976%
5	2.761	520	535	553	rBV4	32710	80374	2.07%	0.636%
6	3.908	880	892	915	rBV2	80132	272267	7.02%	2.153%
7	4.342	1013	1027	1053	rVB	108627	282065	7.27%	2.230%
8	5.040	1228	1244	1265	rBV2	254527	625722	16.13%	4.947%
9	5.613	1410	1422	1445	rBV	207445	432172	11.14%	3.417%
10	5.905	1498	1513	1536	rBV	1672356	3201766	82.54%	25.316%
11	6.066	1551	1563	1582	rBV	150681	307295	7.92%	2.430%
12	6.985	1837	1849	1869	rBV	63814	131289	3.38%	1.038%
13	7.310	1937	1950	1972	rBV	273326	491054	12.66%	3.883%
14	7.622	2037	2047	2061	rBV2	33850	64827	1.67%	0.513%
15	7.969	2137	2155	2177	rBV	2312567	3879103	100.00%	30.671%
16	8.092	2183	2193	2231	rVB	285258	637596	16.44%	5.041%
17	8.847	2416	2428	2446	rBV	319488	535436	13.80%	4.234%
18	10.210	2838	2852	2867	rBV	98619	163524	4.22%	1.293%
19	11.243	3162	3173	3192	rBV	295244	496775	12.81%	3.928%
20	11.616	3278	3289	3310	rVV	245379	413263	10.65%	3.268%




Sum of corrected areas: 12647327

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101822\
Data File : VV028615.D
Acq On : 18 Oct 2022 15:07
Operator : SY/MD
Sample : N5173-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXS7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

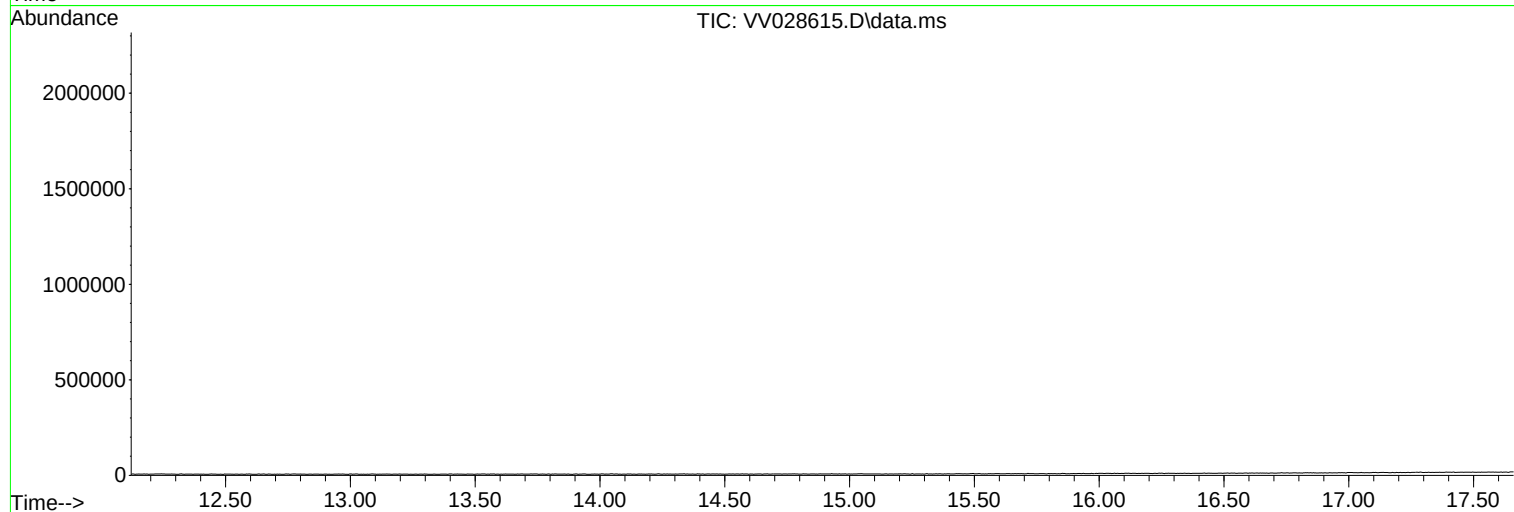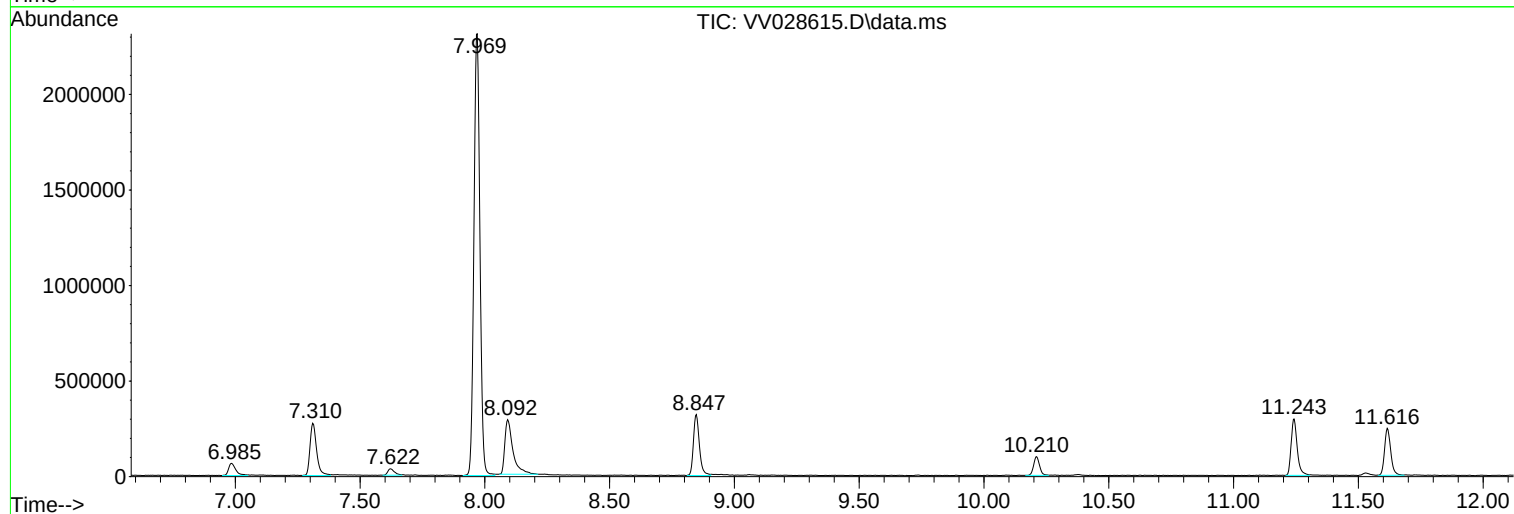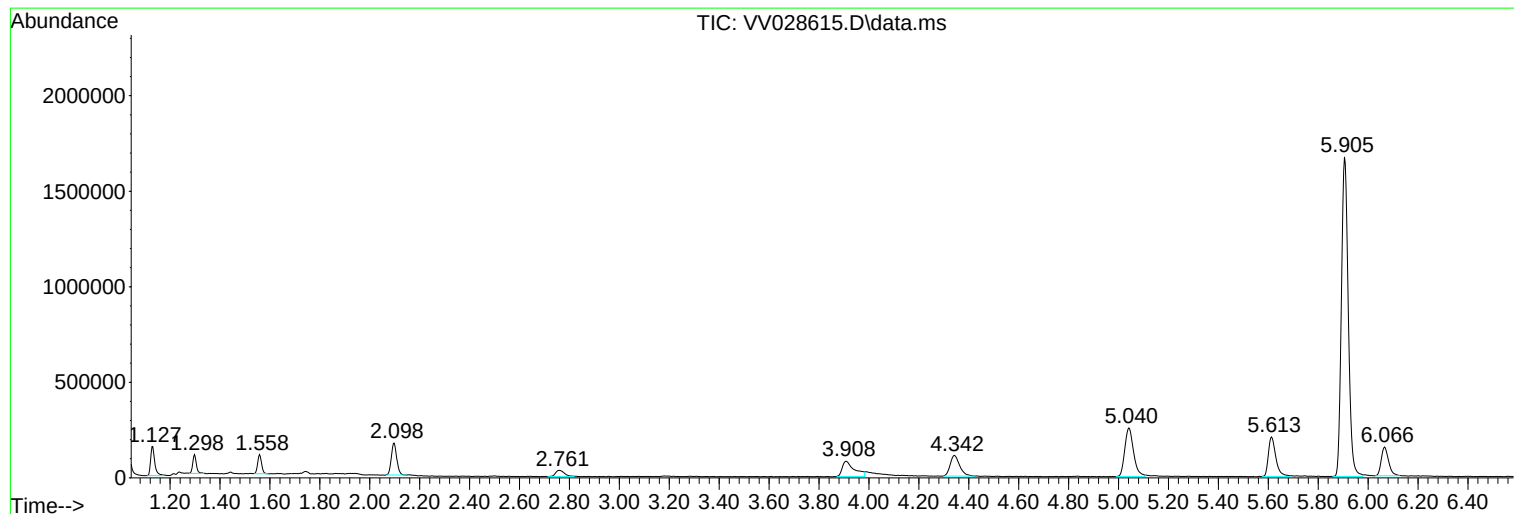

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101822\
Data File : VV028615.D
Acq On : 18 Oct 2022 15:07
Operator : SY/MD
Sample : N5173-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXS7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101822\
Data File : VV028615.D
Acq On : 18 Oct 2022 15:07
Operator : SY/MD
Sample : N5173-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXS7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------