

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101822\
 Data File : VV028616.D
 Acq On : 18 Oct 2022 15:32
 Operator : SY/MD
 Sample : N5173-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFXS8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028616.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.236	51	61	68	rBV2	18572	29210	1.29%	0.341%
2	1.301	74	81	90	rBV	103699	106225	4.69%	1.240%
3	1.561	155	162	171	rBV	102017	112770	4.98%	1.317%
4	2.101	320	330	350	rVB	178365	270352	11.94%	3.157%
5	2.770	522	538	551	rBV	27207	59611	2.63%	0.696%
6	3.912	876	893	928	rBV3	73581	289708	12.79%	3.383%
7	4.342	1013	1027	1054	rBV2	111416	298506	13.18%	3.486%
8	5.043	1228	1245	1274	rBV2	268249	679566	30.01%	7.935%
9	5.612	1411	1422	1441	rBV	197092	411832	18.19%	4.809%
10	5.908	1499	1514	1545	rBV	1154250	2264259	100.00%	26.439%
11	6.066	1550	1563	1585	rVV	161351	337508	14.91%	3.941%
12	6.985	1836	1849	1868	rBV	66559	133672	5.90%	1.561%
13	7.313	1939	1951	1970	rBV	288619	519455	22.94%	6.066%
14	7.622	2038	2047	2064	rBV2	36658	68821	3.04%	0.804%
15	7.969	2134	2155	2173	rBV	429615	728518	32.17%	8.507%
16	8.088	2183	2192	2228	rBV	307643	654740	28.92%	7.645%
17	8.847	2417	2428	2447	rBV	301230	505808	22.34%	5.906%
18	10.210	2840	2852	2865	rBV	106430	169546	7.49%	1.980%
19	11.242	3161	3173	3194	rBV	286865	464819	20.53%	5.428%
20	11.529	3250	3262	3277	rBV4	18206	37112	1.64%	0.433%
21	11.615	3277	3289	3308	rVV	259025	421962	18.64%	4.927%




Sum of corrected areas: 8564000

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101822\
Data File : VV028616.D
Acq On : 18 Oct 2022 15:32
Operator : SY/MD
Sample : N5173-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXS8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

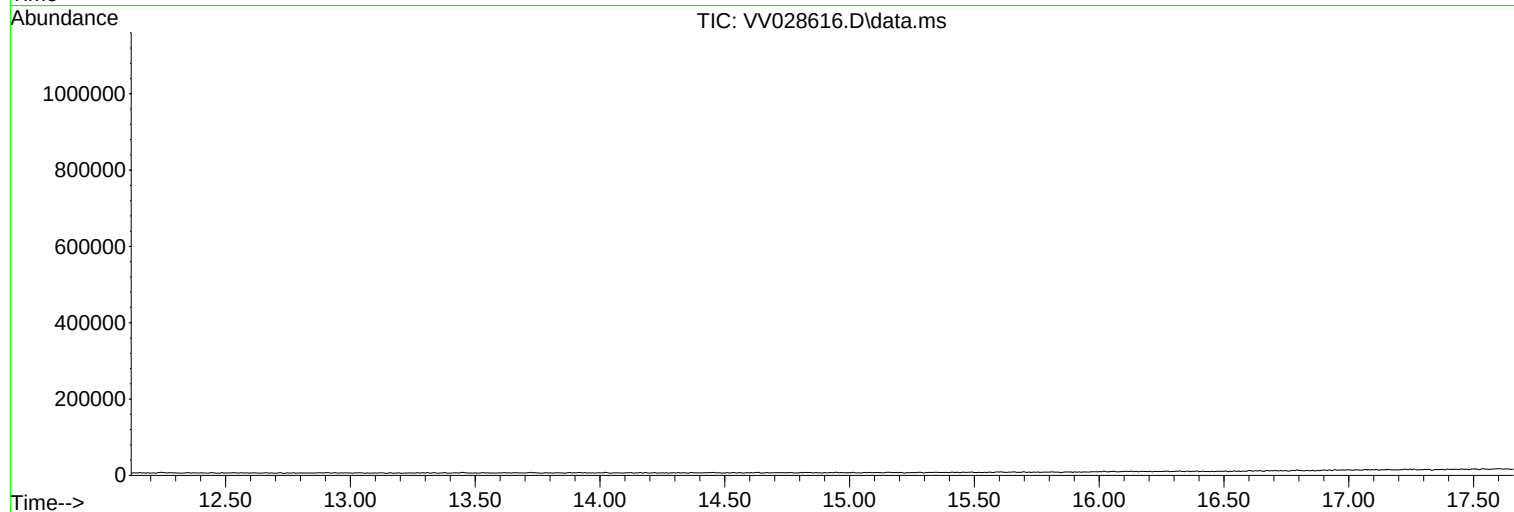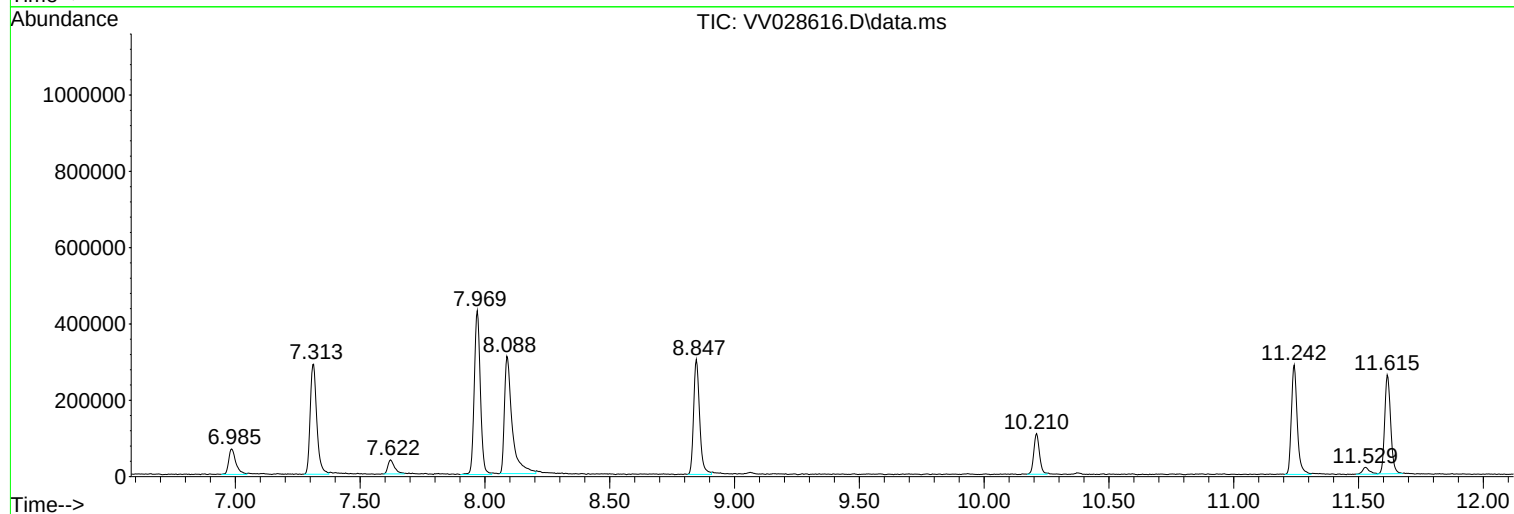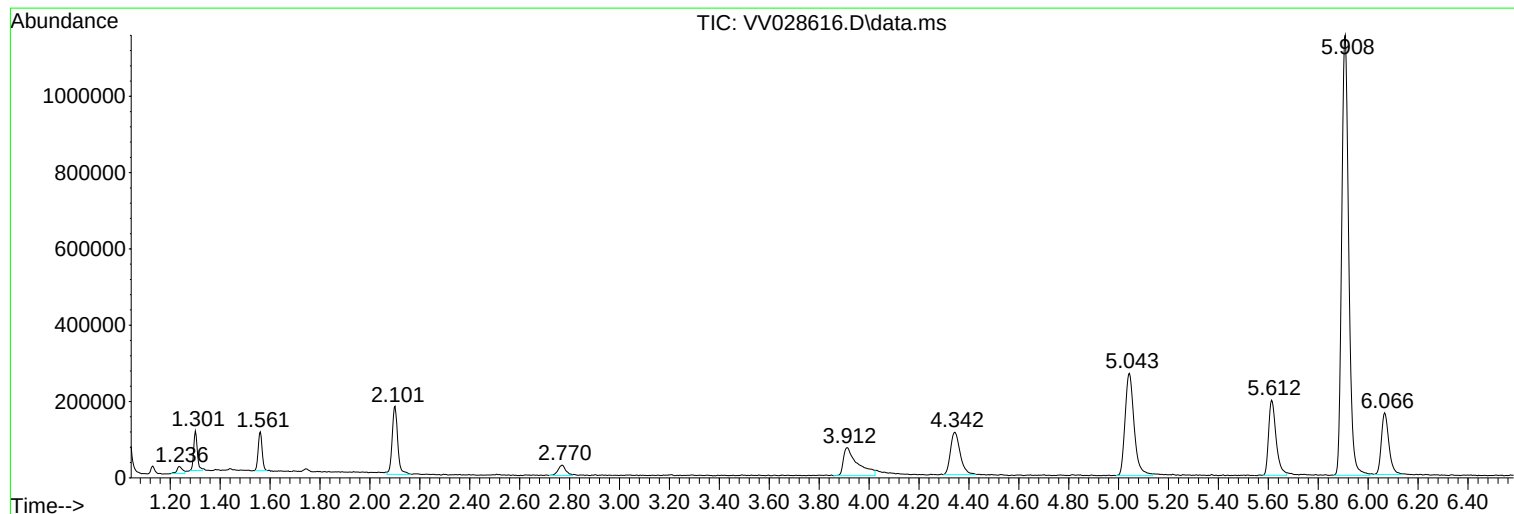

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101822\
Data File : VV028616.D
Acq On : 18 Oct 2022 15:32
Operator : SY/MD
Sample : N5173-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXS8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101822\
Data File : VV028616.D
Acq On : 18 Oct 2022 15:32
Operator : SY/MD
Sample : N5173-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXS8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc