

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101822\
 Data File : VV028617.D
 Acq On : 18 Oct 2022 15:57
 Operator : SY/MD
 Sample : N5173-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFXS9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028617.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.127	21	27	37	rBV2	55385	61143	1.33%	0.416%
2	1.294	74	79	92	rVB	95636	99389	2.16%	0.676%
3	1.558	154	161	174	rVB	101267	115127	2.50%	0.783%
4	1.741	210	218	229	rVB	144535	183810	3.99%	1.249%
5	2.098	318	329	342	rBV3	201469	316622	6.87%	2.152%
6	2.770	526	538	551	rVB4	18644	50951	1.11%	0.346%
7	3.896	874	888	900	rBV	192015	501355	10.88%	3.408%
8	4.336	1009	1025	1049	rVB	117365	302865	6.57%	2.059%
9	5.034	1227	1242	1265	rBV2	279667	641850	13.93%	4.363%
10	5.609	1406	1421	1441	rBV	223681	452589	9.82%	3.076%
11	5.902	1494	1512	1534	rBV	2203010	4220597	91.60%	28.688%
12	6.063	1549	1562	1581	rVB	157644	320517	6.96%	2.179%
13	6.986	1838	1849	1867	rBV	64113	123150	2.67%	0.837%
14	7.310	1939	1950	1974	rBV	275377	486405	10.56%	3.306%
15	7.622	2037	2047	2063	rVB2	33220	63820	1.39%	0.434%
16	7.966	2136	2154	2174	rBV	2780576	4607621	100.00%	31.319%
17	8.098	2185	2195	2225	rBV	277899	599529	13.01%	4.075%
18	8.844	2416	2427	2444	rBV	322113	532527	11.56%	3.620%
19	10.210	2839	2852	2868	rBV	97779	161122	3.50%	1.095%
20	11.239	3162	3172	3196	rBV	294860	479528	10.41%	3.259%
21	11.616	3279	3289	3307	rVB	244170	391432	8.50%	2.661%




Sum of corrected areas: 14711949

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101822\
Data File : VV028617.D
Acq On : 18 Oct 2022 15:57
Operator : SY/MD
Sample : N5173-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXS9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

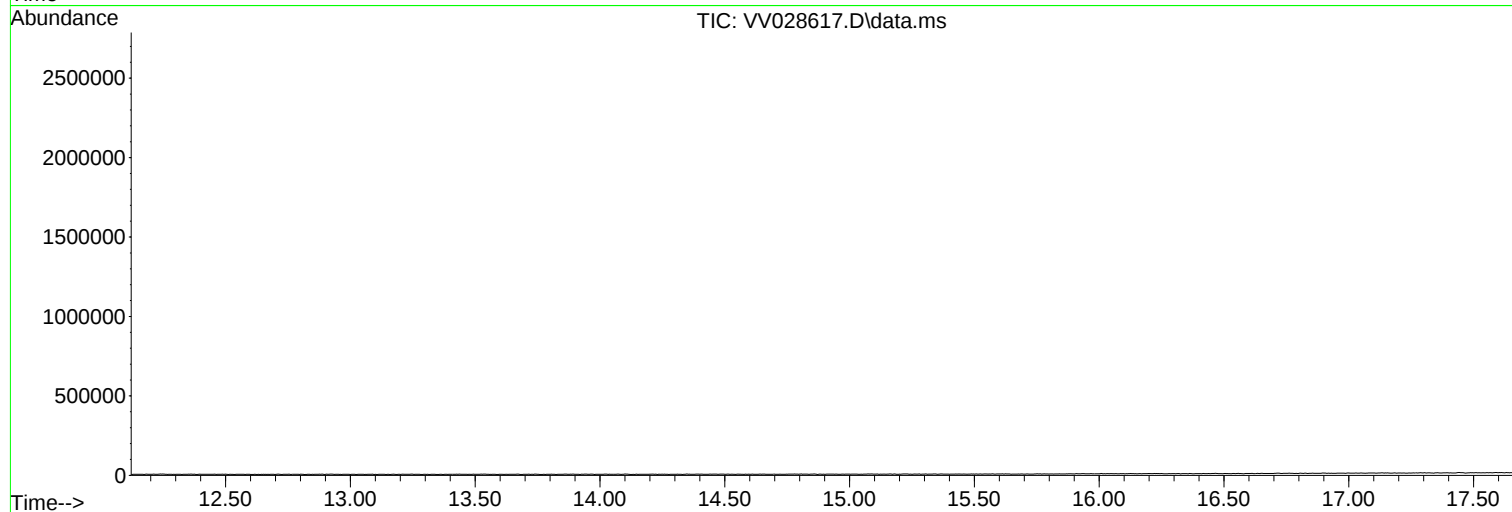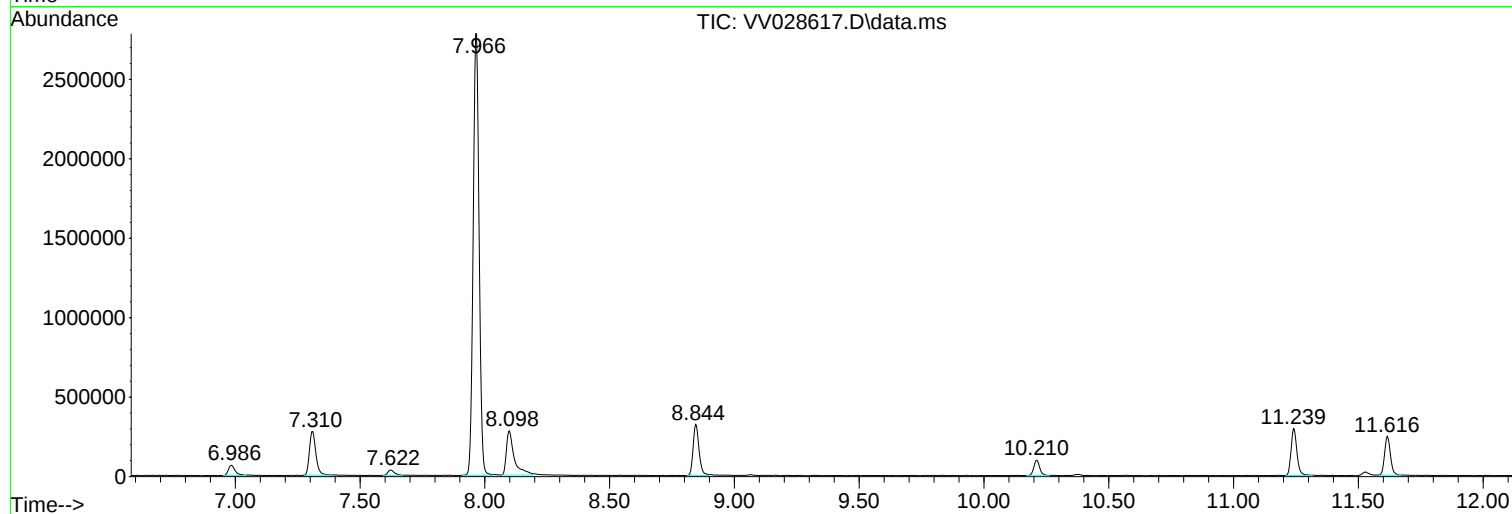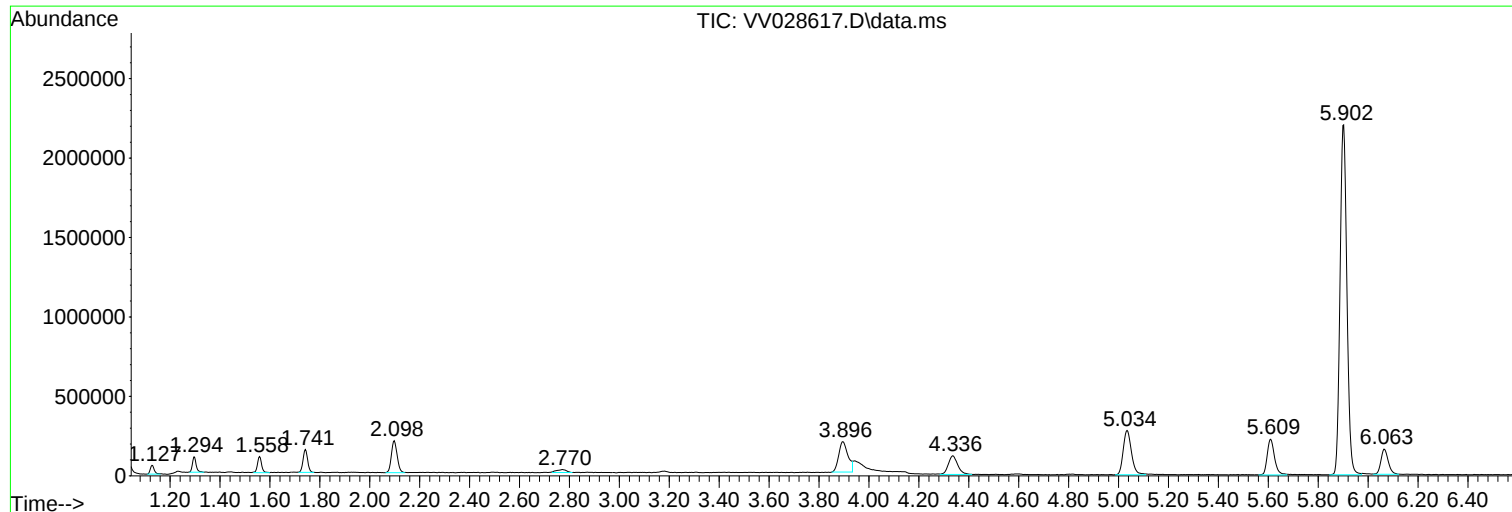

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101822\
Data File : VV028617.D
Acq On : 18 Oct 2022 15:57
Operator : SY/MD
Sample : N5173-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXS9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101822\
Data File : VV028617.D
Acq On : 18 Oct 2022 15:57
Operator : SY/MD
Sample : N5173-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXS9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc