

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101822\
 Data File : VV028620.D
 Acq On : 18 Oct 2022 17:58
 Operator : SY/MD
 Sample : N5103-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028620.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.237	54	61	64	rBV8	5298	7172	1.10%	0.131%
2	1.301	75	81	93	rVB	91053	94944	14.52%	1.732%
3	1.565	155	163	173	rVB	95950	110326	16.87%	2.013%
4	2.102	321	330	343	rBV	164915	237428	36.31%	4.331%
5	2.507	444	456	462	rBV3	11213	19796	3.03%	0.361%
6	3.912	876	893	930	rBV2	50649	243324	37.21%	4.439%
7	4.343	1012	1027	1048	rBV2	111384	278743	42.63%	5.085%
8	5.040	1228	1244	1274	rBV2	260934	653891	100.00%	11.929%
9	5.613	1411	1422	1454	rBV	218607	452792	69.25%	8.260%
10	6.066	1549	1563	1582	rBV	159327	329538	50.40%	6.012%
11	6.986	1836	1849	1863	rBV2	64940	125258	19.16%	2.285%
12	7.310	1938	1950	1967	rBV	283274	501936	76.76%	9.157%
13	7.622	2037	2047	2061	rBV2	35916	68166	10.42%	1.244%
14	7.934	2133	2144	2146	rBV10	5486	7096	1.09%	0.129%
15	8.088	2183	2192	2226	rBV	302978	651652	99.66%	11.888%
16	8.847	2416	2428	2446	rBV	329973	554097	84.74%	10.108%
17	10.211	2841	2852	2866	rBV	104557	172699	26.41%	3.151%
18	10.381	2896	2905	2914	rVB9	6547	12590	1.93%	0.230%
19	11.239	3157	3172	3191	rBV	304522	504995	77.23%	9.213%
20	11.616	3276	3289	3312	rBV	255979	421636	64.48%	7.692%
21	15.866	4597	4611	4615	rBV	14433	33500	5.12%	0.611%




Sum of corrected areas: 5481579

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101822\
Data File : VV028620.D
Acq On : 18 Oct 2022 17:58
Operator : SY/MD
Sample : N5103-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

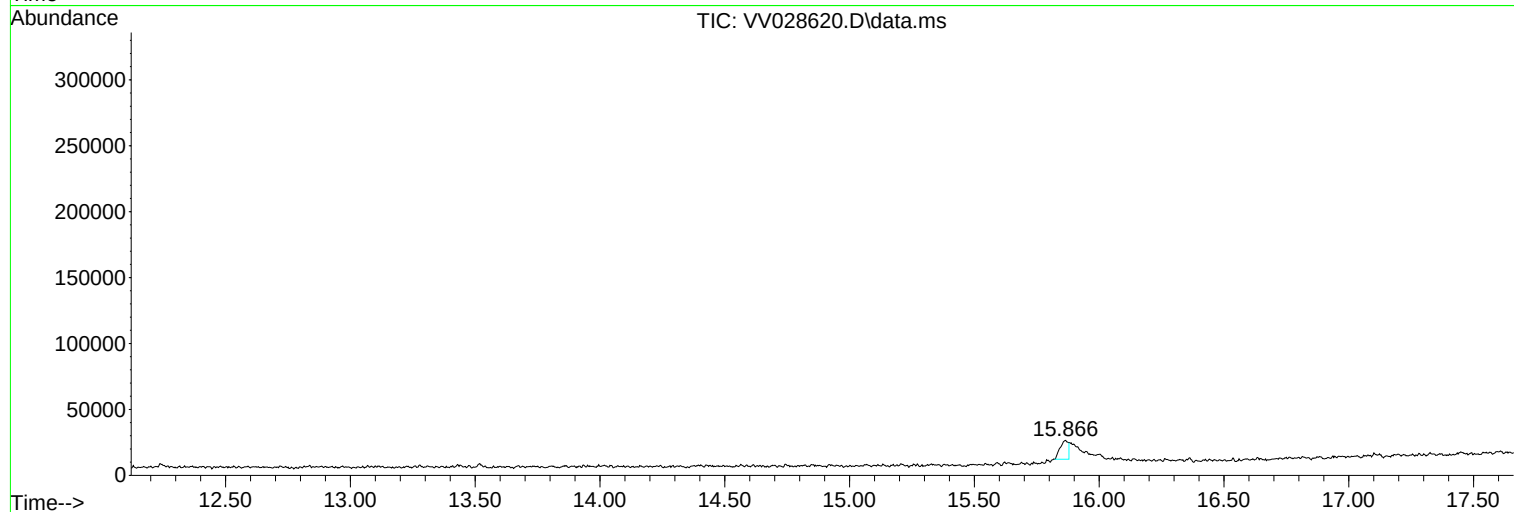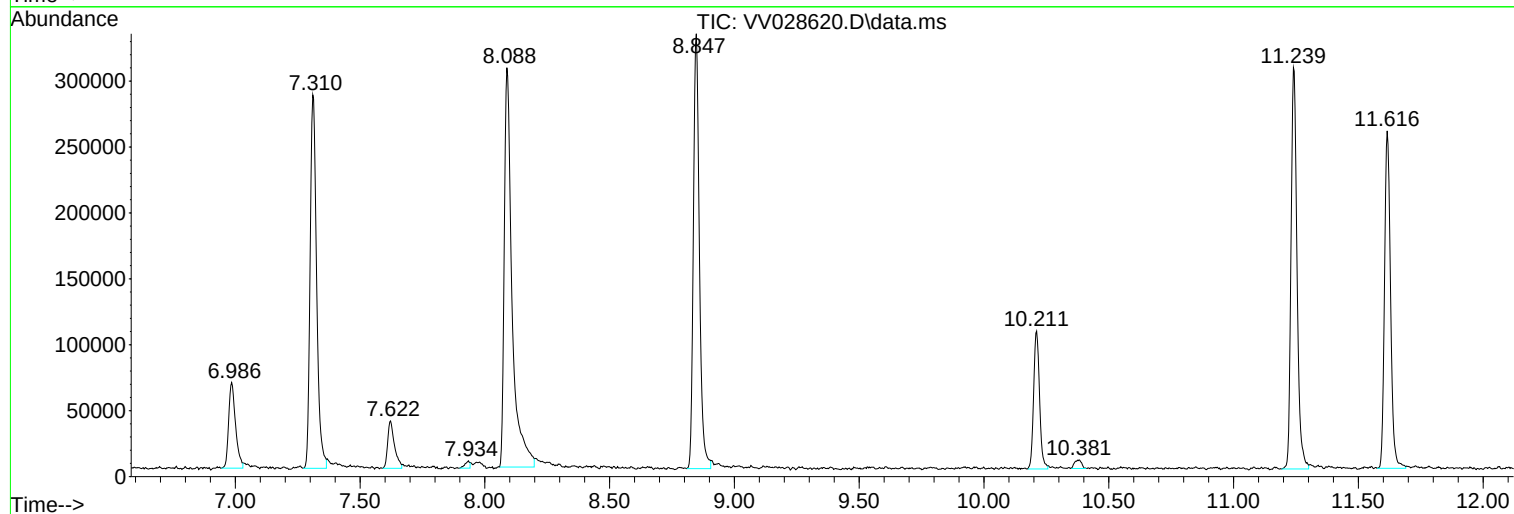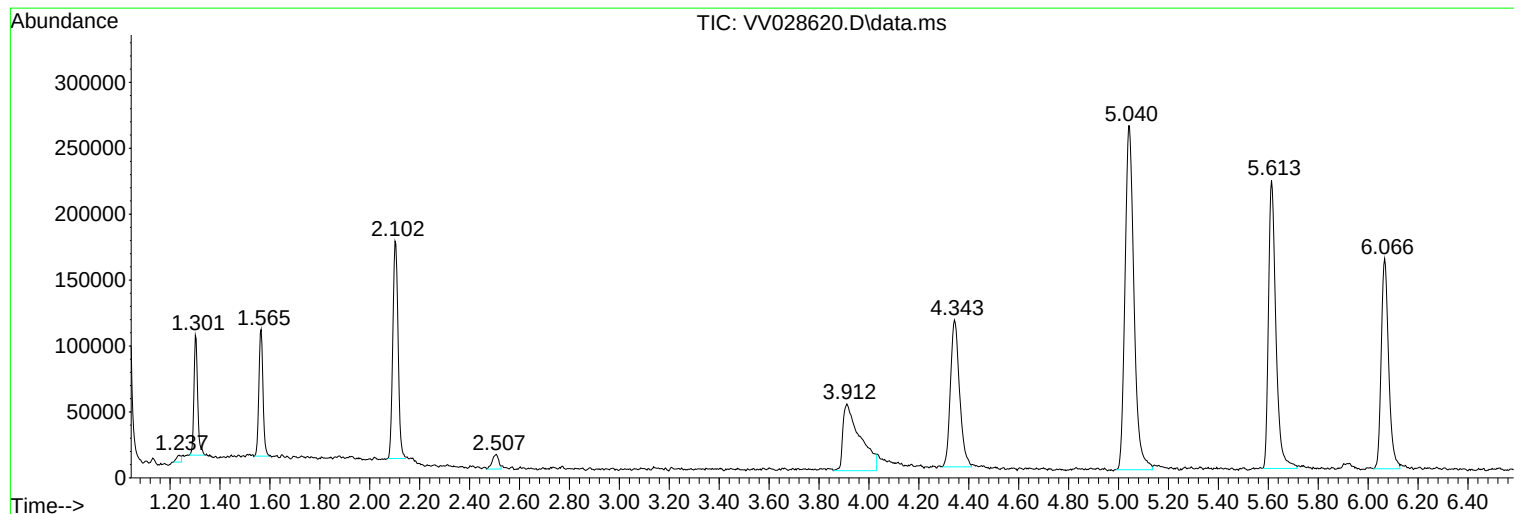

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101822\
Data File : VV028620.D
Acq On : 18 Oct 2022 17:58
Operator : SY/MD
Sample : N5103-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101822\
Data File : VV028620.D
Acq On : 18 Oct 2022 17:58
Operator : SY/MD
Sample : N5103-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc