

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101822\
 Data File : VV028624.D
 Acq On : 18 Oct 2022 19:37
 Operator : SY/MD
 Sample : VIBLK301
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK301

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028624.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.224	47	57	59	rBV4	11196	14105	1.81%	0.253%
2	1.294	73	79	93	rBV	89395	91247	11.71%	1.634%
3	1.555	153	160	174	rVB	91812	105143	13.49%	1.883%
4	2.095	319	328	340	rVB	156514	218548	28.04%	3.913%
5	2.494	446	452	461	rVB3	13995	21975	2.82%	0.394%
6	3.940	882	902	935	rBV2	87246	353332	45.33%	6.327%
7	4.342	1013	1027	1048	rVB	124554	309984	39.77%	5.551%
8	4.850	1177	1185	1186	rBV8	22098	28147	3.61%	0.504%
9	5.030	1229	1241	1258	rBV3	372018	779480	100.00%	13.958%
10	5.583	1403	1413	1430	rVB	284835	591901	75.94%	10.599%
11	6.047	1547	1557	1573	rVB	188104	361158	46.33%	6.467%
12	6.989	1840	1850	1864	rVB	83365	139816	17.94%	2.504%
13	7.313	1940	1951	1967	rBV	293054	495350	63.55%	8.870%
14	7.436	1985	1989	1998	rVB	24713	17175	2.20%	0.308%
15	7.625	2037	2048	2061	rVB2	36600	64465	8.27%	1.154%
16	8.114	2187	2200	2231	rBV	279061	564864	72.47%	10.115%
17	8.850	2417	2429	2450	rBV	292285	478242	61.35%	8.564%
18	10.214	2842	2853	2867	rBV	87465	140023	17.96%	2.507%
19	11.242	3162	3173	3193	rBV	277664	433450	55.61%	7.762%
20	11.615	3278	3289	3305	rBV	209787	343529	44.07%	6.152%
21	15.844	4592	4604	4607	rBV9	18021	32537	4.17%	0.583%




Sum of corrected areas: 5584471

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101822\
Data File : VV028624.D
Acq On : 18 Oct 2022 19:37
Operator : SY/MD
Sample : VIBLK301
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK301

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

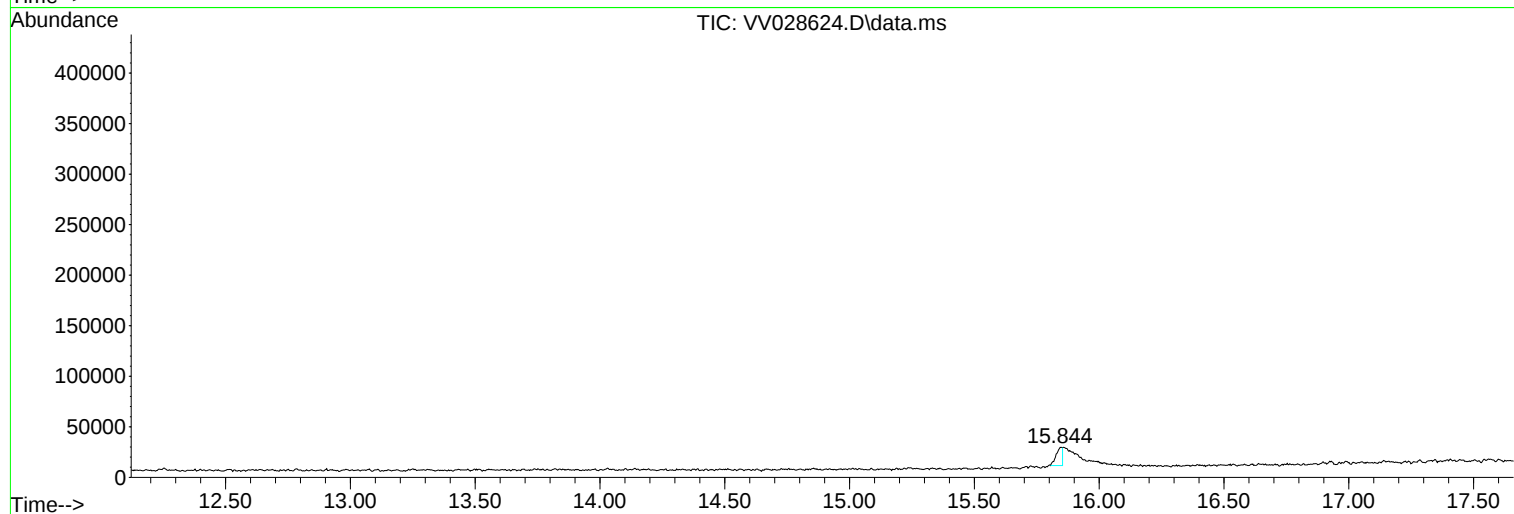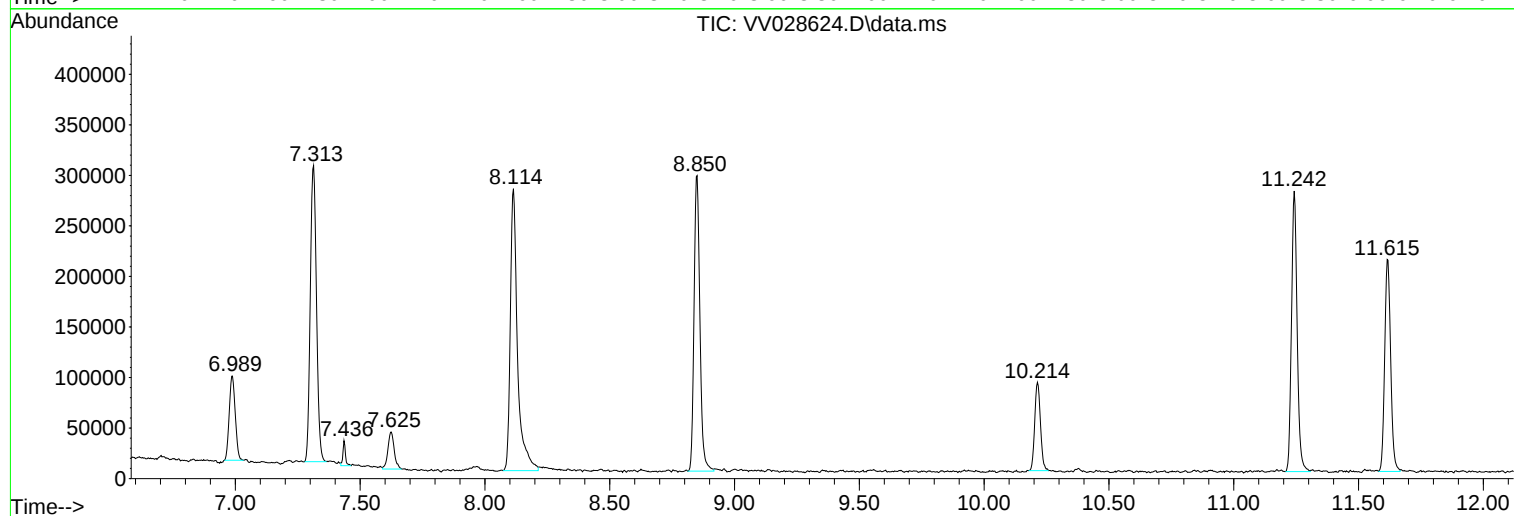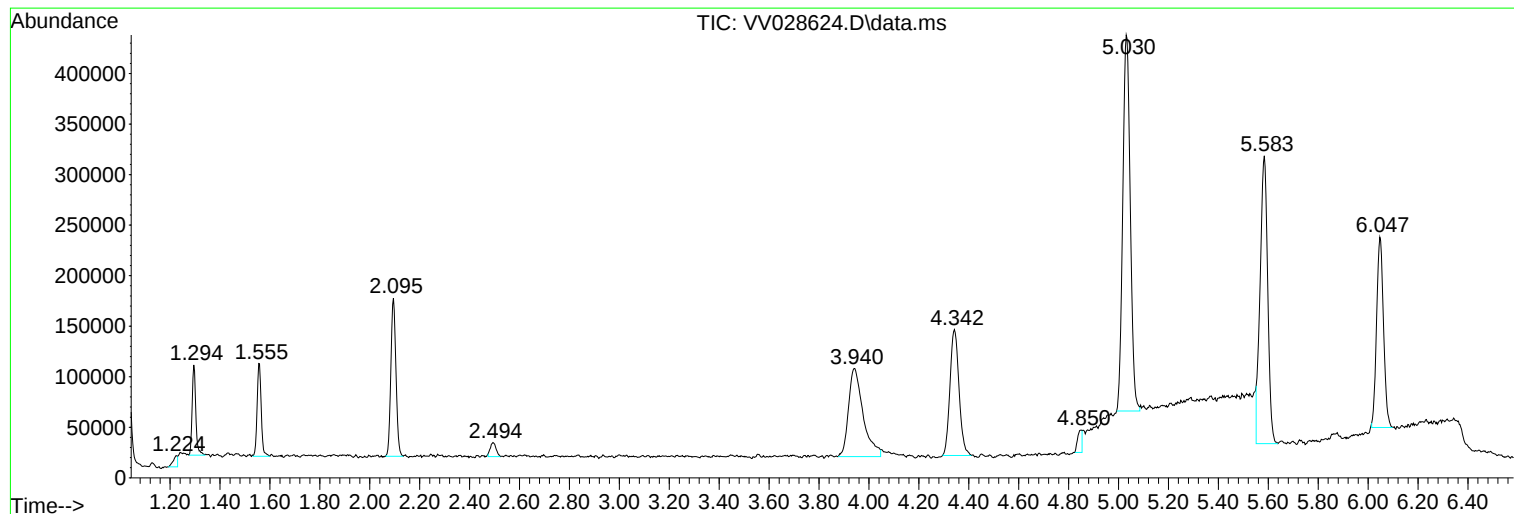

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101822\
Data File : VV028624.D
Acq On : 18 Oct 2022 19:37
Operator : SY/MD
Sample : VIBLK301
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK301

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101822\
Data File : VV028624.D
Acq On : 18 Oct 2022 19:37
Operator : SY/MD
Sample : VIBLK301
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK301

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc