




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101823\
 Data File : VV032479.D
 Acq On : 18 Oct 2023 18:22
 Operator : SY/MD
 Sample : 04944-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49F4

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 10/19/2023
 Supervised By :Mahesh Dadoda 10/20/2023

Quant Time: Oct 19 04:34:43 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 19 04:26:22 2023
 Response via : Initial Calibration

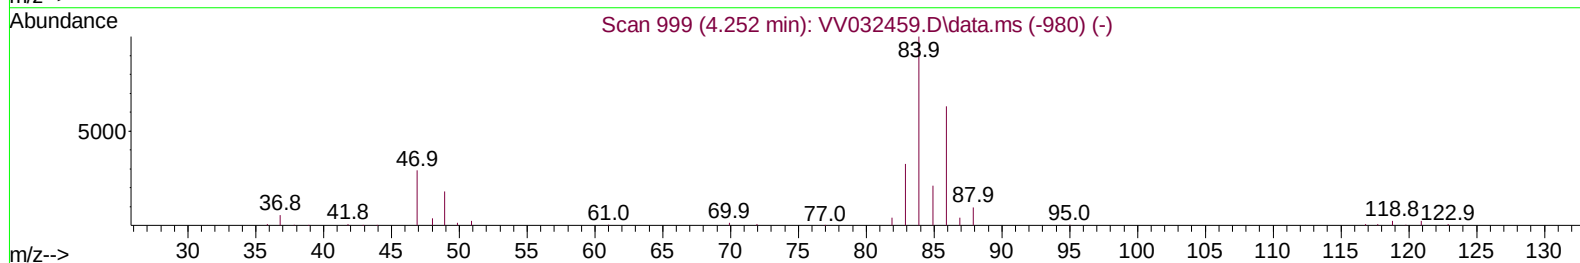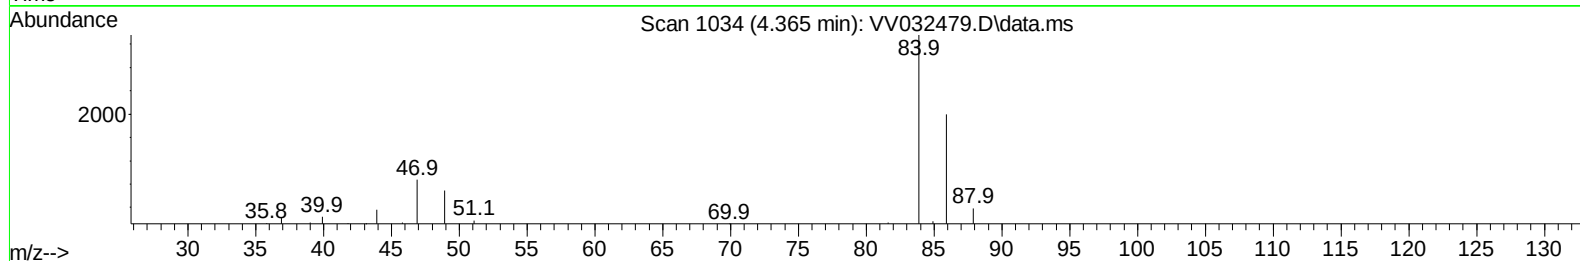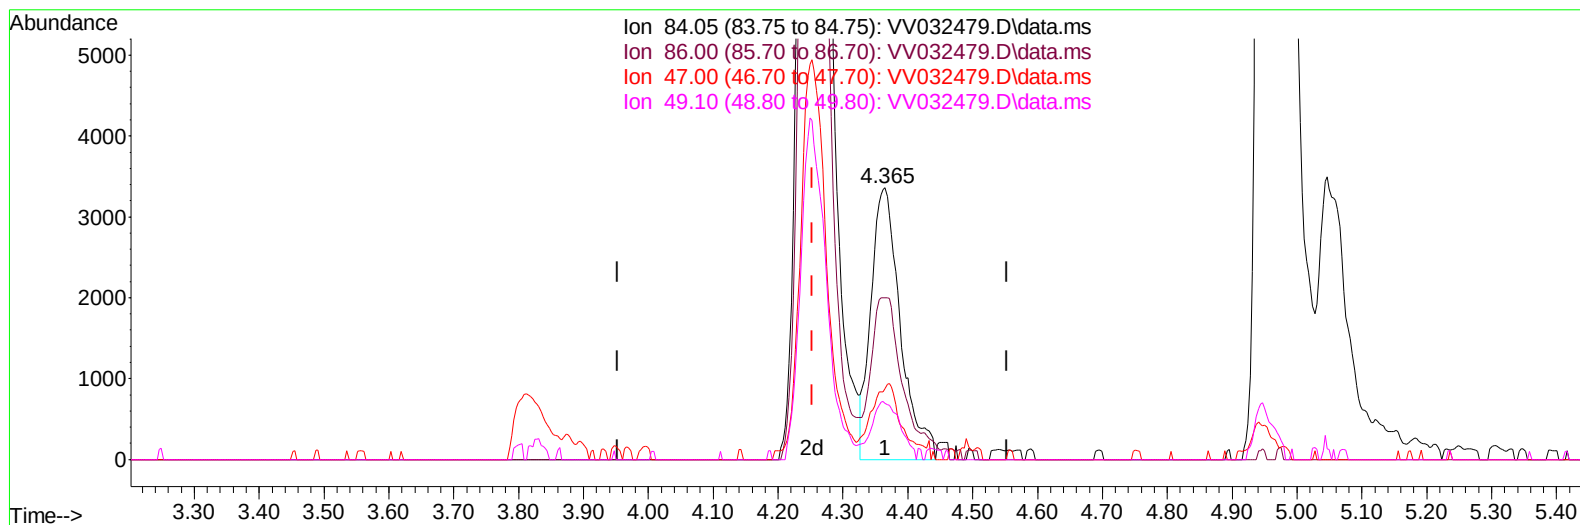

TIC: VV032479.D\data.ms

(24) Chloroform-d (S)

4.365min (+ 0.113) 0.82 ug/L

response 10579

Ion	Exp%	Act%
84.05	100.00	100.00
86.00	61.90	59.08
47.00	43.10	30.24
49.10	25.00	21.14




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101823\
Data File : VV032479.D
Acq On : 18 Oct 2023 18:22
Operator : SY/MD
Sample : 04944-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49F4

Manual IntegrationsAPPROVED

Quant Time: Oct 19 04:34:43 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Oct 19 04:26:22 2023
Response via : Initial Calibration

Reviewed By :John Carlone 10/19/2023
Supervised By :Mahesh Dadoda 10/20/2023

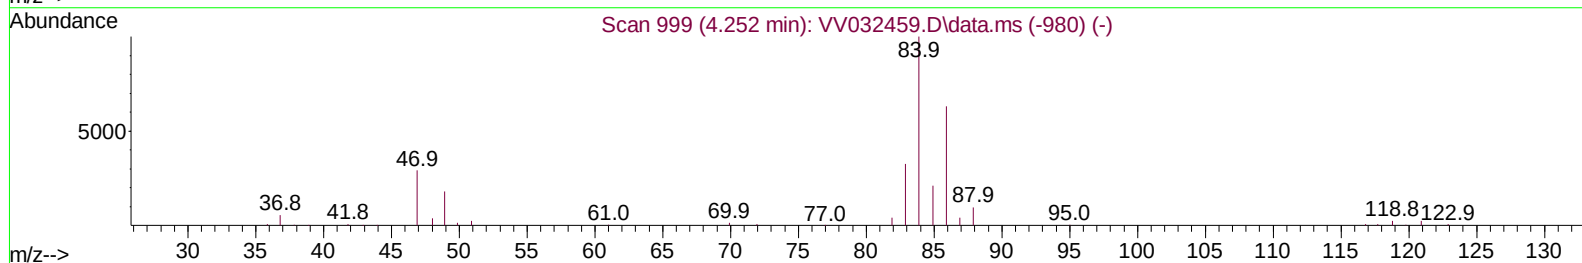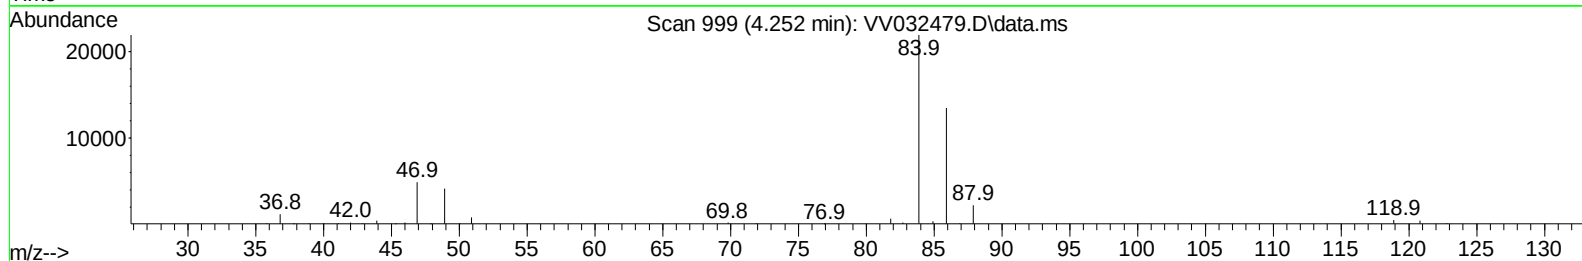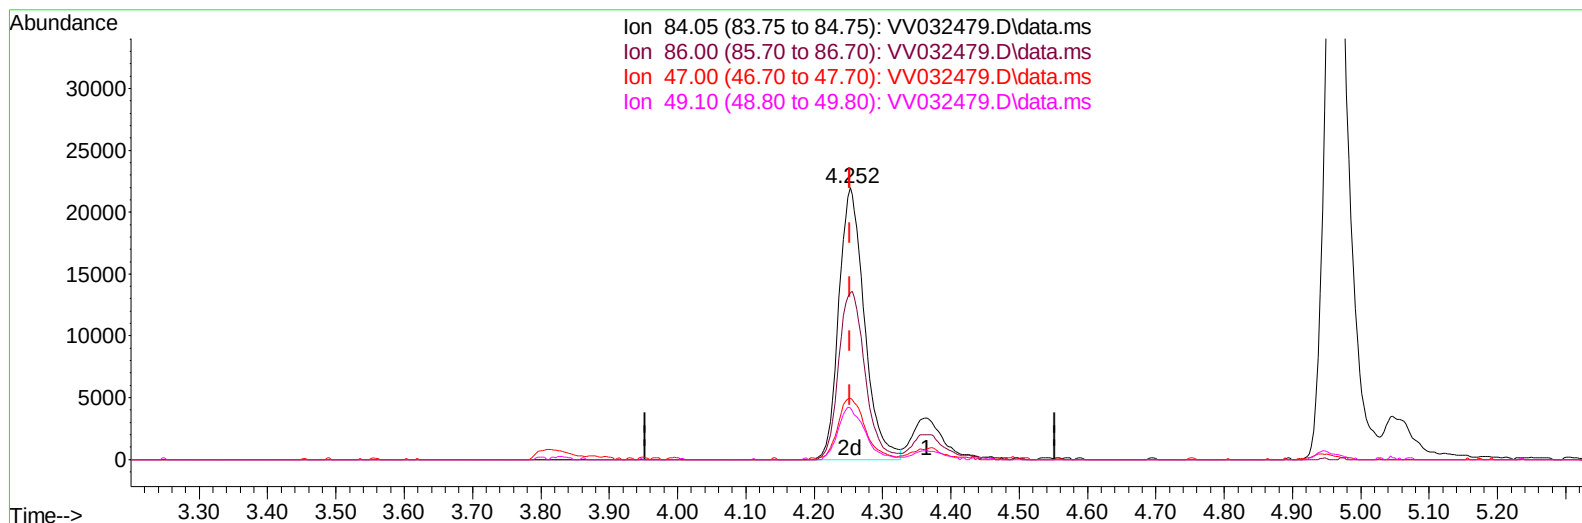

TIC: VV032479.D\data.ms

(24) Chloroform-d (S)

4.252min (+ 0.000) 4.44 ug/L m

response 57012

Ion	Exp%	Act%
84.05	100.00	100.00
86.00	61.90	10.96#
47.00	43.10	5.61#
49.10	25.00	3.92#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101823\
 Data File : VV032479.D
 Acq On : 18 Oct 2023 18:22
 Operator : SY/MD
 Sample : 04944-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49F4

Manual IntegrationsAPPROVED

Reviewed By : John Carlone 10/19/2023
 Supervised By : Mahesh Dadoda 10/20/2023

Quant Time: Oct 19 04:34:43 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 19 04:26:22 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.539	114		89450	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117		102576	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152		45862	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.278	65		37078	5.097	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	102.000%	
7) Chloroethane-d5	1.532	69		32308	5.471	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	109.400%	
11) 1,1-Dichloroethene-d2	2.060	65		13069	4.260	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	85.200%	
20) 2-Butanone-d5	3.809	46		80119	43.536	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	87.080%	
24) Chloroform-d	4.252	84		57012m	4.442	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.800%	
26) 1,2-Dichloroethane-d4	4.947	65		29837	4.908	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.200%	
32) Benzene-d6	4.963	84		121189	4.015	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	80.400%	
36) 1,2-Dichloropropane-d6	5.992	67		39355	3.935	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	78.800%	
41) Toluene-d8	7.246	98		105162	3.810	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	76.200%	
43) trans-1,3-Dichloroprop...	7.561	79		13250	3.739	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	74.800%	
46) 2-Hexanone-d5	8.030	63		64291	38.560	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	77.120%	
56) 1,1,2,2-Tetrachloroeth...	10.156	84		30644	4.381	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	87.600%	
66) 1,2-Dichlorobenzene-d4	11.564	152		38481	4.522	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	90.400%	
Target Compounds							
13) Acetone	2.140	43		2606	1.837	ug/L	Qvalue 91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101823\
Data File : VV032479.D
Acq On : 18 Oct 2023 18:22
Operator : SY/MD
Sample : 04944-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49F4

Manual IntegrationsAPPROVED

Quant Time: Oct 19 04:34:43 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Oct 19 04:26:22 2023
Response via : Initial Calibration

Reviewed By :John Carlone 10/19/2023
Supervised By :Mahesh Dadoda 10/20/2023

