

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101823\
 Data File : VV032475.D
 Acq On : 18 Oct 2023 16:44
 Operator : SY/MD
 Sample : 04944-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49S8

Quant Time: Oct 19 04:33:48 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 19 04:26:22 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	98795	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	108591	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	48185	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	41463	5.160	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	103.200%	
7) Chloroethane-d5	1.532	69	35219	5.400	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	108.000%	
11) 1,1-Dichloroethene-d2	2.060	65	15330	4.524	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	90.400%	
20) 2-Butanone-d5	3.806	46	90560	44.555	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	89.100%	
24) Chloroform-d	4.252	84	62190	4.388	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	87.800%	
26) 1,2-Dichloroethane-d4	4.947	65	33113	4.932	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	98.600%	
32) Benzene-d6	4.963	84	133285	4.171	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	83.400%	
36) 1,2-Dichloropropane-d6	5.989	67	43254	4.086	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	81.800%	
41) Toluene-d8	7.246	98	119796	4.100	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	82.000%	
43) trans-1,3-Dichloroprop...	7.558	79	15046	4.011	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	80.200%	
46) 2-Hexanone-d5	8.027	63	76155	43.146	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	86.300%	
56) 1,1,2,2-Tetrachloroeth...	10.156	84	34267	4.628	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	92.600%	
66) 1,2-Dichlorobenzene-d4	11.564	152	43958	4.916	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	98.400%	
Target Compounds						Qvalue
3) Chloromethane	1.217	50	9555	0.861	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101823\
Data File : VV032475.D
Acq On : 18 Oct 2023 16:44
Operator : SY/MD
Sample : 04944-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49S8

Quant Time: Oct 19 04:33:48 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Oct 19 04:26:22 2023
Response via : Initial Calibration

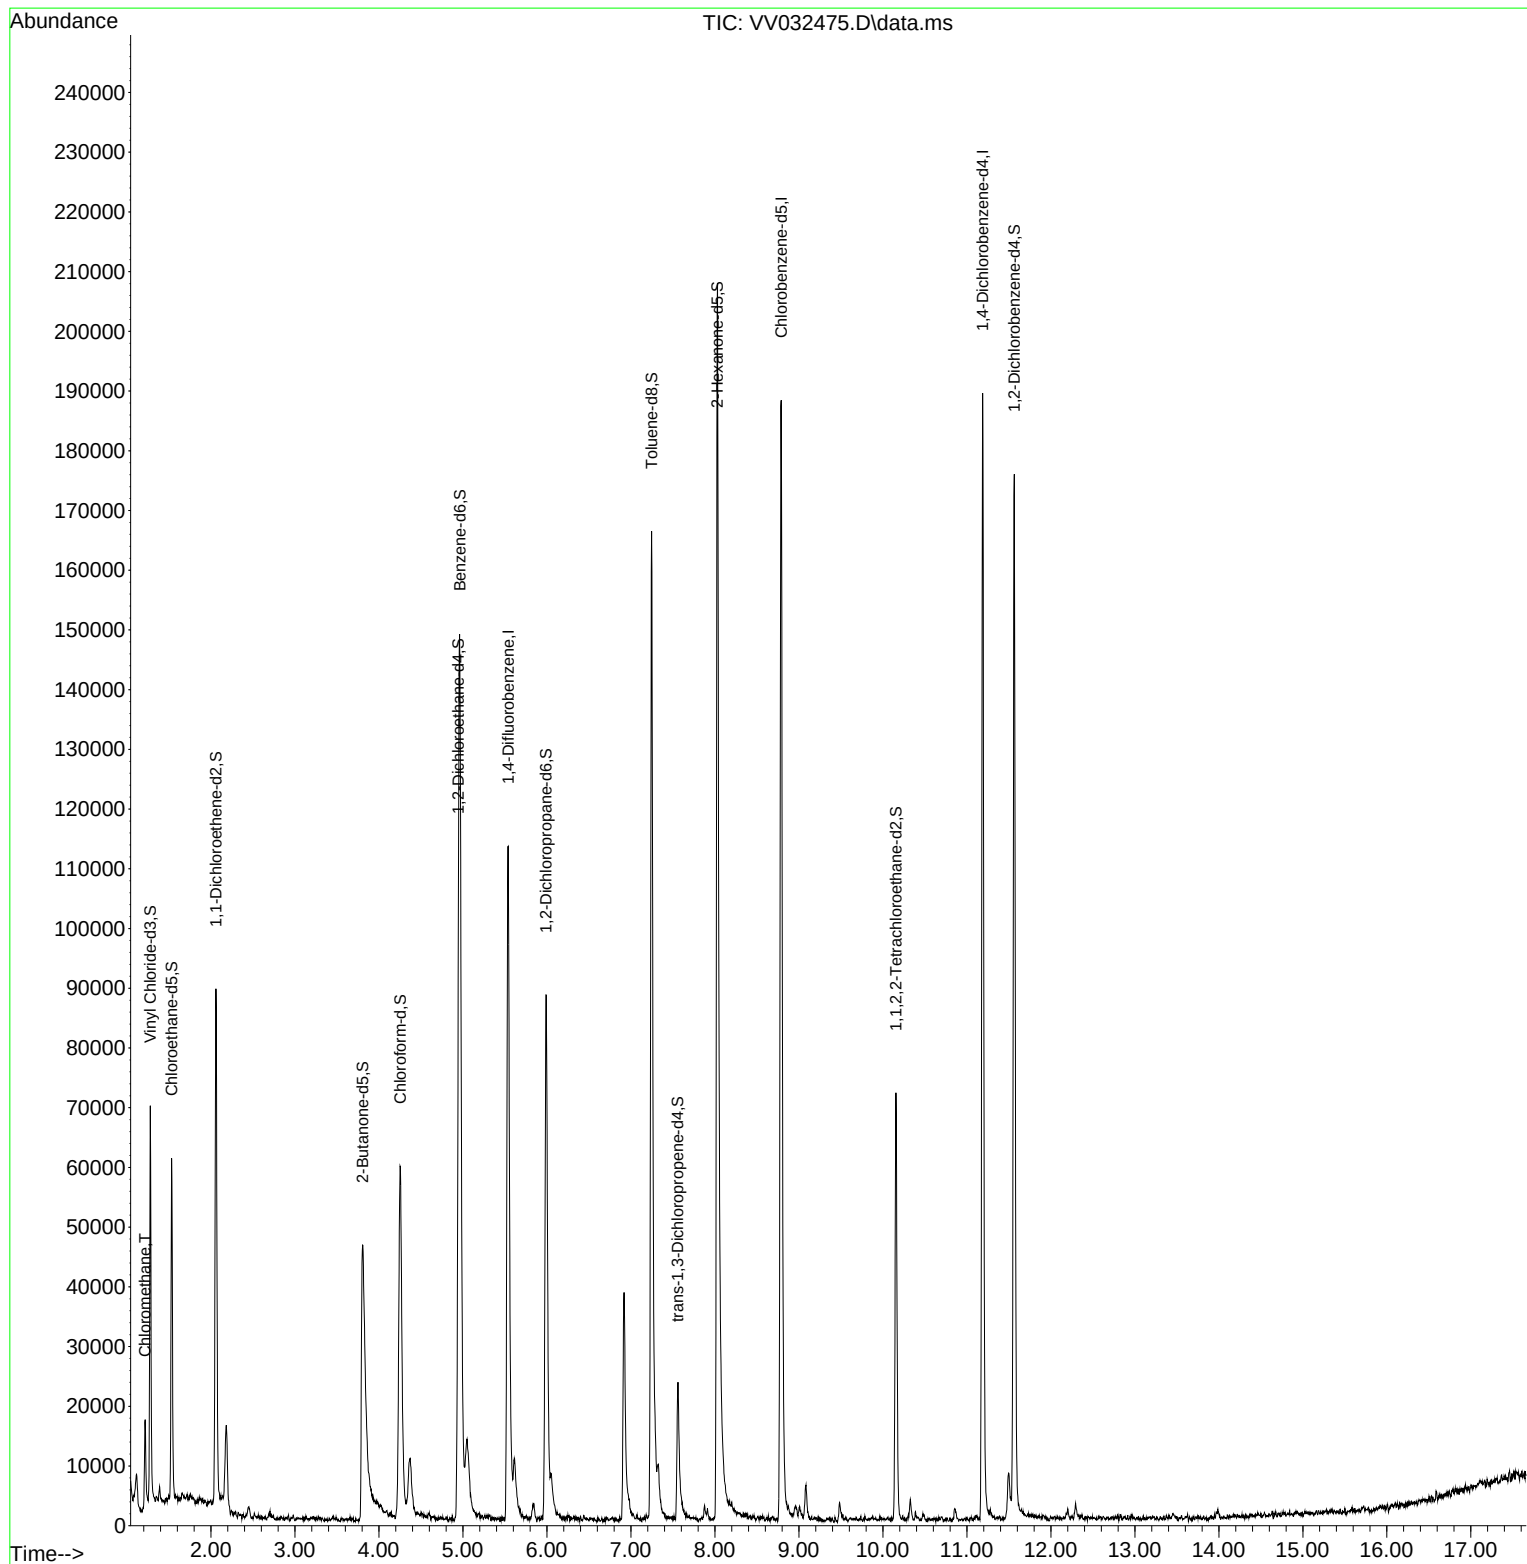

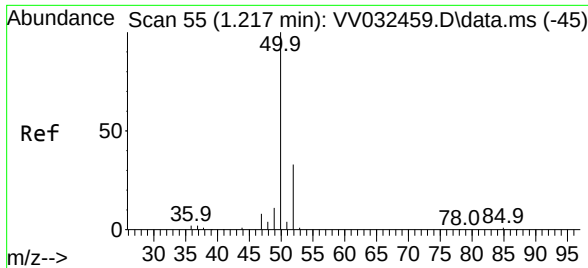

#3
 Chloromethane
 Concen: 0.861 ug/L
 RT: 1.217 min Scan# 51
 Delta R.T. 0.000 min
 Lab File: VV032475.D
 Acq: 18 Oct 2023 16:44

Instrument :
 MSVOA_V
 ClientSampleId :
 A49S8

Tgt Ion: 50 Resp: 9555
 Ion Ratio Lower Upper
 50 100
 52 35.4 23.0 42.6

