

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW101823\
 Data File : VW032476.D
 Acq On : 18 Oct 2023 17:09
 Operator : SY/MD
 Sample : 04944-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49T0

Quant Time: Oct 19 04:34:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 19 04:26:22 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	91835	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	101540	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	46248	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	38331	5.132	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	102.600%
7) Chloroethane-d5	1.532	69	33787	5.573	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	111.400%
11) 1,1-Dichloroethene-d2	2.060	65	13618	4.323	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	86.400%
20) 2-Butanone-d5	3.802	46	82791	43.819	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	87.640%
24) Chloroform-d	4.252	84	58641	4.451	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.000%
26) 1,2-Dichloroethane-d4	4.947	65	30137	4.829	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.600%
32) Benzene-d6	4.963	84	125485	4.200	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.000%
36) 1,2-Dichloropropane-d6	5.992	67	40138	4.055	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	81.000%
41) Toluene-d8	7.246	98	109050	3.991	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.800%
43) trans-1,3-Dichloroprop...	7.558	79	13808	3.936	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.800%
46) 2-Hexanone-d5	8.027	63	70493	42.711	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	85.420%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	32708	4.724	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.400%
66) 1,2-Dichlorobenzene-d4	11.564	152	40818	4.756	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.200%
Target Compounds						
					Qvalue	
13) Acetone	2.130	43	2637	1.811	ug/L	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101823\
Data File : VV032476.D
Acq On : 18 Oct 2023 17:09
Operator : SY/MD
Sample : 04944-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49T0

Quant Time: Oct 19 04:34:02 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Oct 19 04:26:22 2023
Response via : Initial Calibration

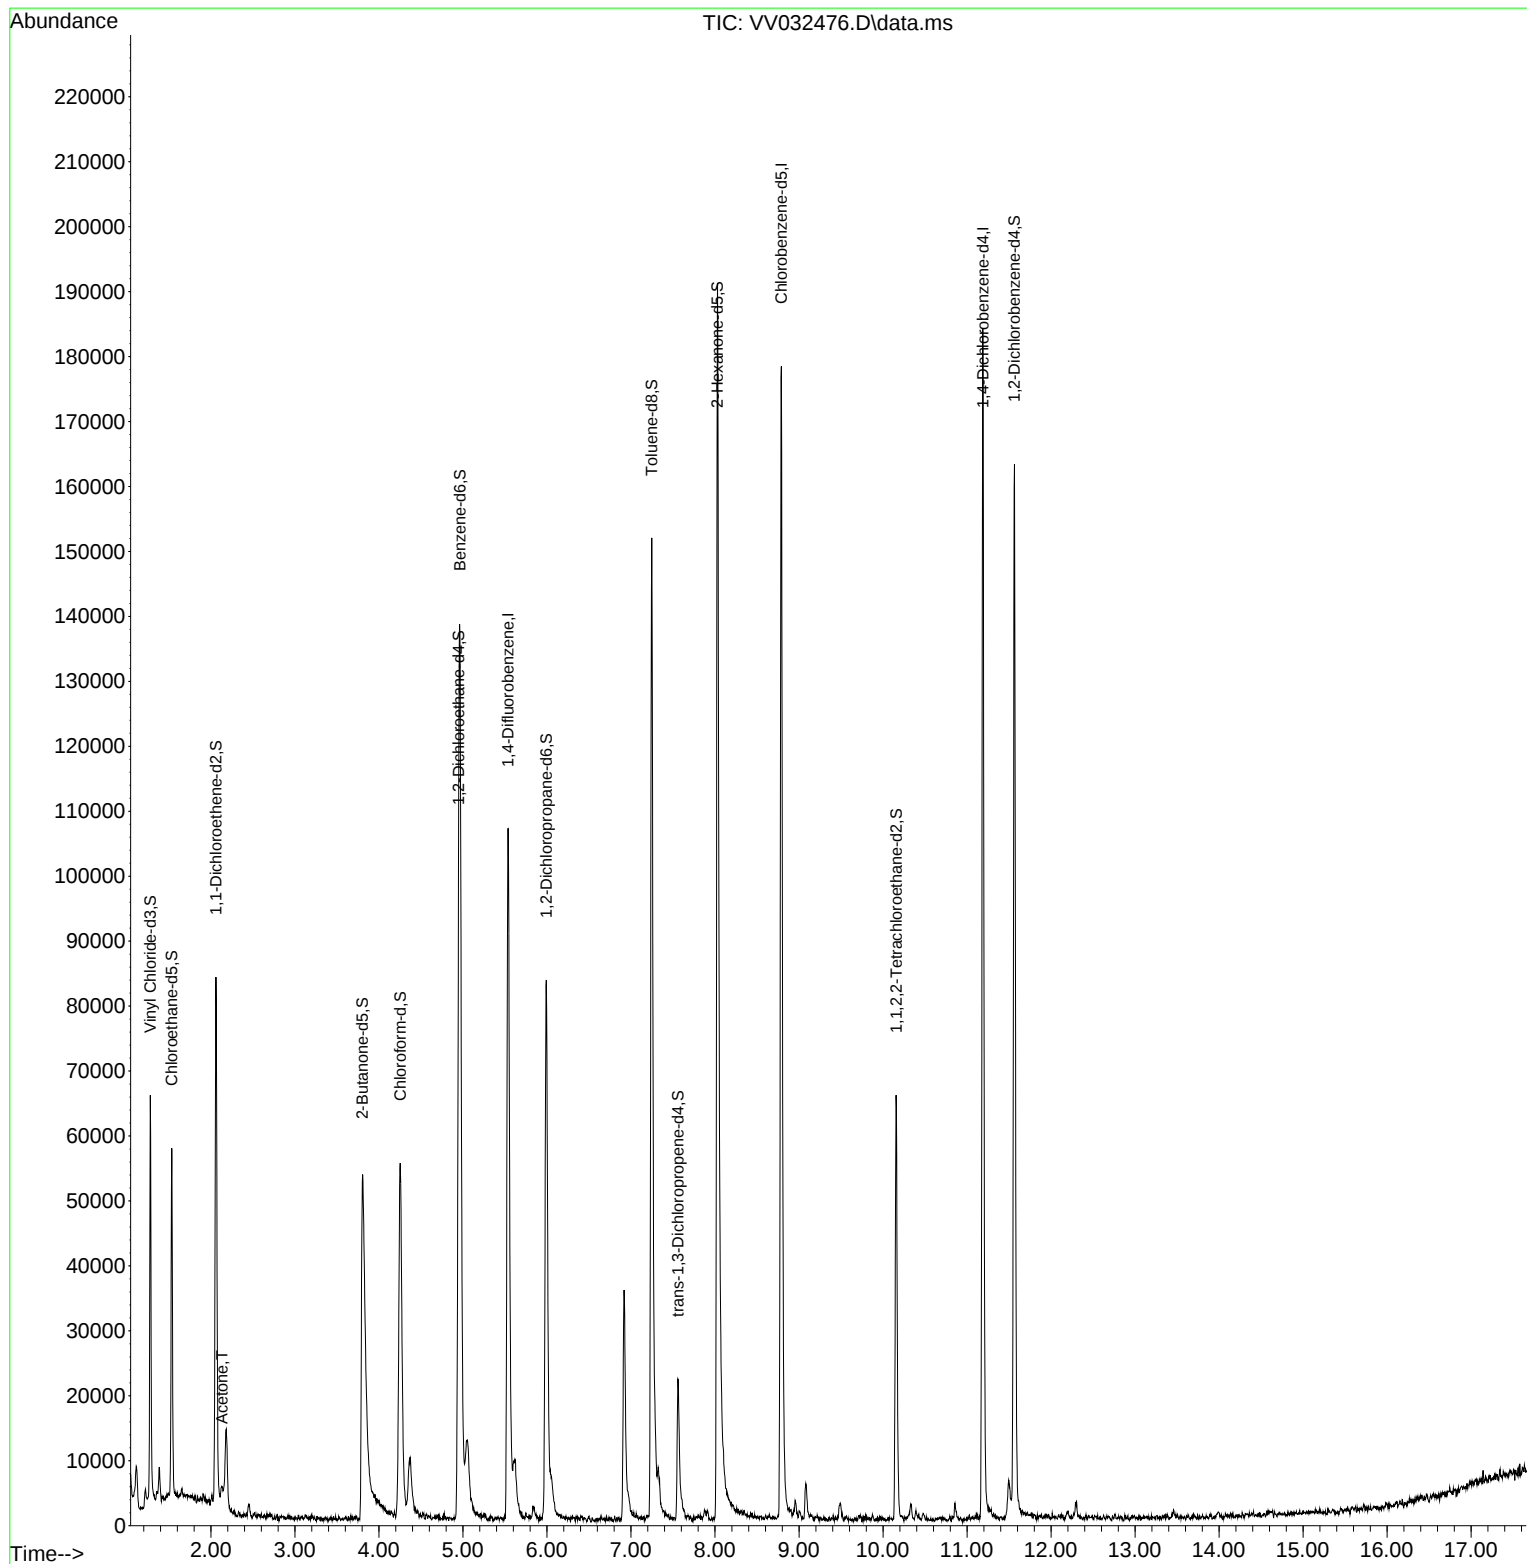

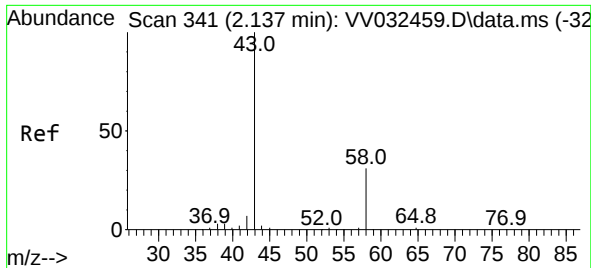

#13
 Acetone
 Concen: 1.811 ug/L
 RT: 2.130 min Scan# 31
 Delta R.T. -0.006 min
 Lab File: VV032476.D
 Acq: 18 Oct 2023 17:09

Instrument :
 MSVOA_V
 ClientSampleId :
 A49T0

Tgt Ion: 43 Resp: 2637
 Ion Ratio Lower Upper
 43 100
 58 45.3 0.0 66.0

