

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VW101823\  
 Data File : VW032482.D  
 Acq On : 18 Oct 2023 19:34  
 Operator : SY/MD  
 Sample : 04944-10  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 26 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 A49R6

Quant Time: Oct 19 04:35:24 2023  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR092923WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Thu Oct 19 04:26:22 2023  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon  | Response | Conc     | Units | Dev(Min) |
|-------------------------------|--------|-------|----------|----------|-------|----------|
| -----                         |        |       |          |          |       |          |
| Internal Standards            |        |       |          |          |       |          |
| 1) 1,4-Difluorobenzene        | 5.535  | 114   | 97939    | 5.000    | ug/L  | 0.00     |
| 28) Chlorobenzene-d5          | 8.789  | 117   | 102932   | 5.000    | ug/L  | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 11.188 | 152   | 46277    | 5.000    | ug/L  | 0.00     |
| System Monitoring Compounds   |        |       |          |          |       |          |
| 4) Vinyl Chloride-d3          | 1.278  | 65    | 36625    | 4.598    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 40 - 130 | Recovery | =     | 92.000%  |
| 7) Chloroethane-d5            | 1.532  | 69    | 31740    | 4.909    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 65 - 130 | Recovery | =     | 98.200%  |
| 11) 1,1-Dichloroethene-d2     | 2.060  | 65    | 15133    | 4.505    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 60 - 125 | Recovery | =     | 90.000%  |
| 20) 2-Butanone-d5             | 3.806  | 46    | 77981    | 38.701   | ug/L  | 0.00     |
| Spiked Amount                 | 50.000 | Range | 40 - 130 | Recovery | =     | 77.400%  |
| 24) Chloroform-d              | 4.252  | 84    | 62024    | 4.414    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =     | 88.200%  |
| 26) 1,2-Dichloroethane-d4     | 4.947  | 65    | 31301    | 4.703    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =     | 94.000%  |
| 32) Benzene-d6                | 4.963  | 84    | 122399   | 4.041    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =     | 80.800%  |
| 36) 1,2-Dichloropropane-d6    | 5.992  | 67    | 40757    | 4.061    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 60 - 140 | Recovery | =     | 81.200%  |
| 41) Toluene-d8                | 7.246  | 98    | 103266   | 3.729    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =     | 74.600%  |
| 43) trans-1,3-Dichloroprop... | 7.561  | 79    | 13095    | 3.683    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 55 - 130 | Recovery | =     | 73.600%  |
| 46) 2-Hexanone-d5             | 8.030  | 63    | 63621    | 38.026   | ug/L  | 0.00     |
| Spiked Amount                 | 50.000 | Range | 45 - 130 | Recovery | =     | 76.060%  |
| 56) 1,1,2,2-Tetrachloroeth... | 10.156 | 84    | 30470    | 4.341    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 65 - 120 | Recovery | =     | 86.800%  |
| 66) 1,2-Dichlorobenzene-d4    | 11.564 | 152   | 36717    | 4.276    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 80 - 120 | Recovery | =     | 85.600%  |
| Target Compounds              |        |       |          |          |       |          |
| 13) Acetone                   | 2.127  | 43    | 2675     | 1.722    | ug/L  | 90       |
| -----                         |        |       |          |          |       |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV101823\  
Data File : VV032482.D  
Acq On : 18 Oct 2023 19:34  
Operator : SY/MD  
Sample : 04944-10  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 26 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
A49R6

Quant Time: Oct 19 04:35:24 2023  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR092923WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Thu Oct 19 04:26:22 2023  
Response via : Initial Calibration

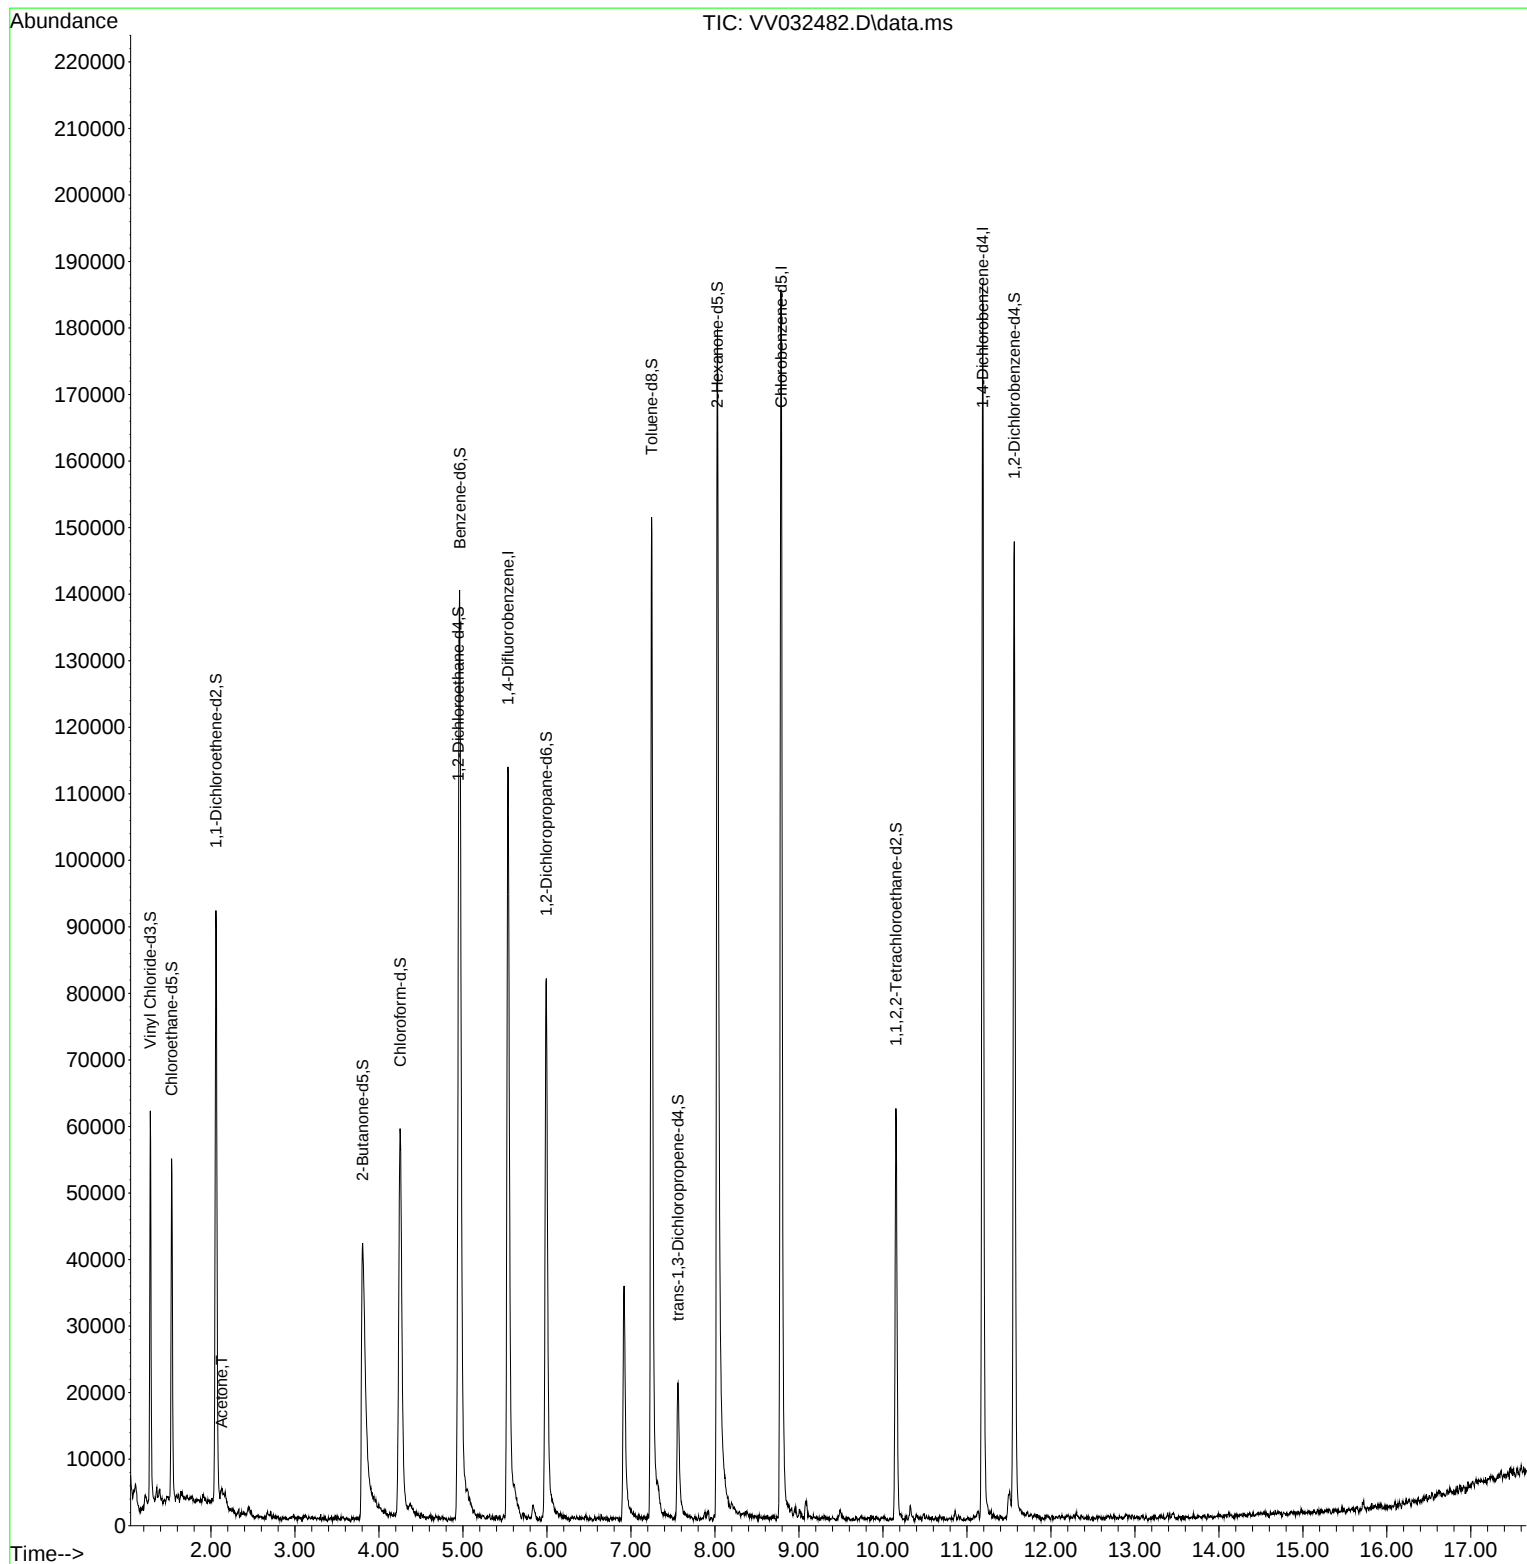

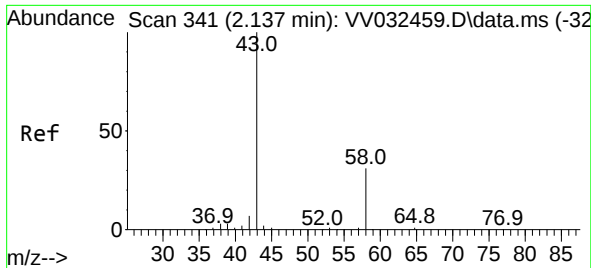

#13

Acetone

Concen: 1.722 ug/L

RT: 2.127 min Scan# 31

Delta R.T. -0.010 min

Lab File: VV032482.D

Acq: 18 Oct 2023 19:34

Instrument :

MSVOA\_V

ClientSampleId :

A49R6

Tgt Ion: 43 Resp: 2675

Ion Ratio Lower Upper

43 100

58 38.5 0.0 66.0

