

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101823\
 Data File : VV032460.D
 Acq On : 18 Oct 2023 10:36
 Operator : SY/MD
 Sample : VV1018WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK372

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032460.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.111	18	22	32	rVB	4395	6128	1.17%	0.171%
2	1.278	67	74	83	rBV	53961	55782	10.61%	1.558%
3	1.532	146	153	167	rVB	49707	58683	11.16%	1.639%
4	2.060	307	317	329	rBV	86048	126409	24.05%	3.530%
5	2.182	346	355	364	rVB4	5630	10155	1.93%	0.284%
6	2.455	428	440	445	rBV6	4430	7530	1.43%	0.210%
7	3.828	854	867	899	rBV2	39705	178144	33.89%	4.975%
8	4.256	982	1000	1024	rBV	65226	174793	33.25%	4.881%
9	4.963	1202	1220	1238	rBV2	148494	379383	72.17%	10.594%
10	5.539	1386	1399	1415	rBV	127858	270216	51.40%	7.546%
11	5.834	1480	1491	1499	rBV10	3973	8028	1.53%	0.224%
12	5.995	1527	1541	1554	rBV	87465	187334	35.64%	5.231%
13	6.921	1818	1829	1853	rBV	34670	80803	15.37%	2.256%
14	7.246	1917	1930	1954	rBV	161742	318859	60.66%	8.904%
15	7.561	2018	2028	2050	rBV2	22231	47988	9.13%	1.340%
16	8.034	2164	2175	2209	rBV	236107	525692	100.00%	14.680%
17	8.789	2399	2410	2433	rBV	209011	370356	70.45%	10.342%
18	9.079	2493	2500	2513	rBV3	5338	10994	2.09%	0.307%
19	10.159	2824	2836	2852	rBV	76096	125571	23.89%	3.507%
20	11.188	3146	3156	3176	rBV	210744	339497	64.58%	9.481%
21	11.564	3262	3273	3288	rBV	178237	290610	55.28%	8.115%
22	13.448	3852	3859	3872	rVB2	4852	7999	1.52%	0.223%




Sum of corrected areas: 3580954

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101823\
Data File : VV032460.D
Acq On : 18 Oct 2023 10:36
Operator : SY/MD
Sample : VV1018WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK372

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

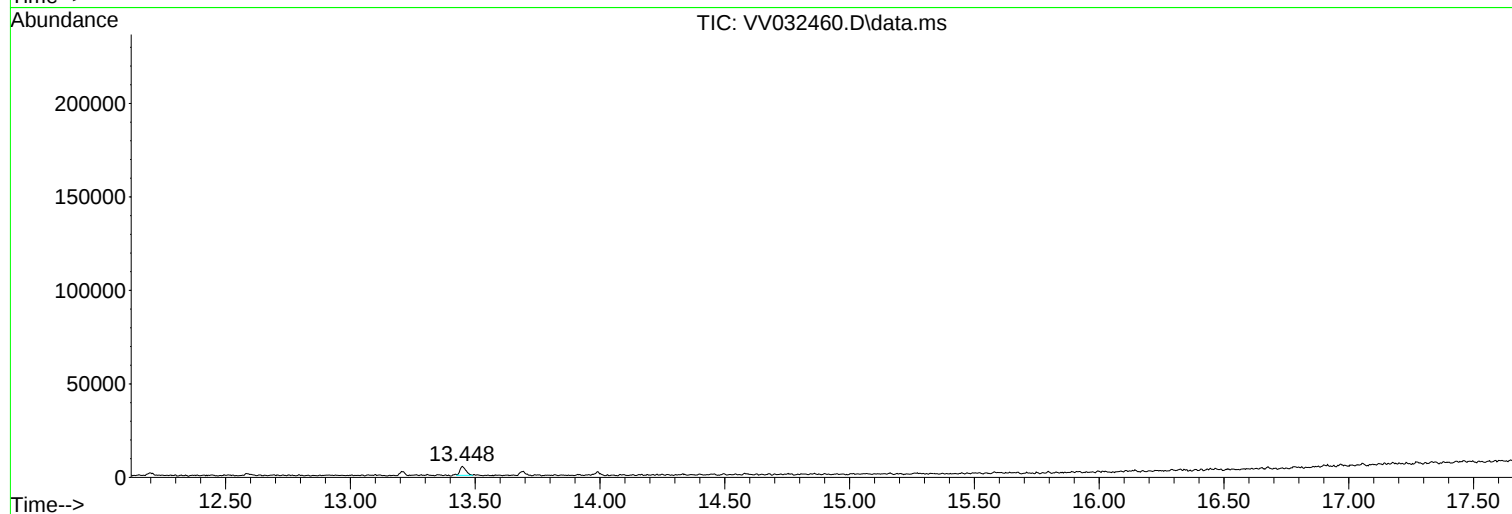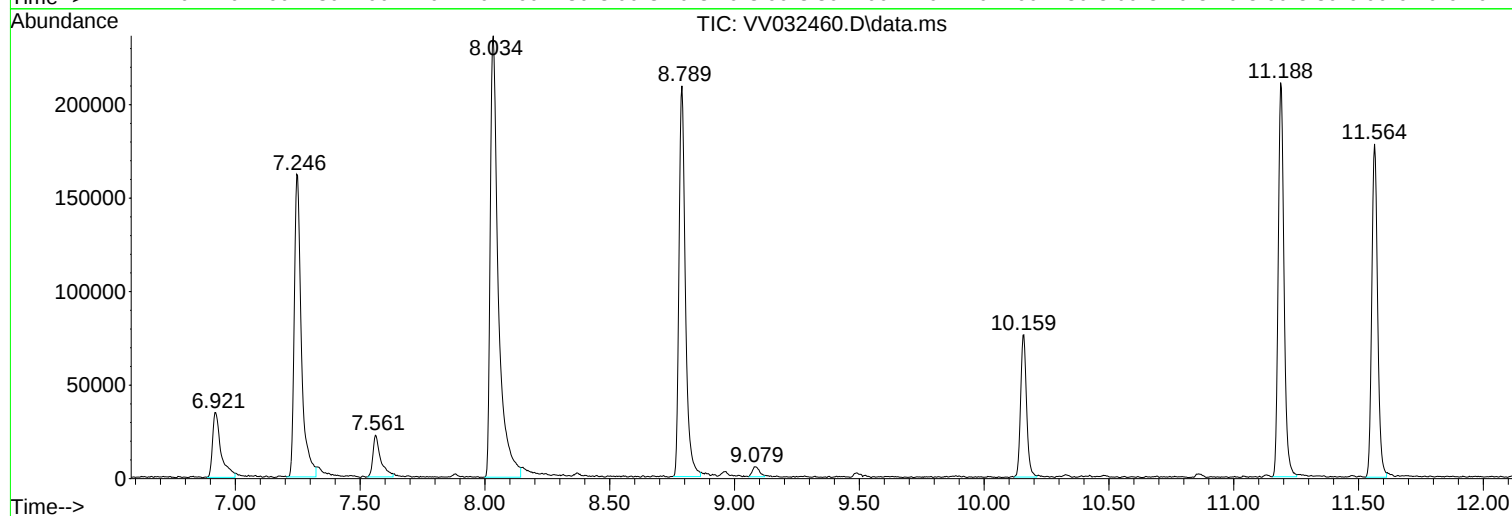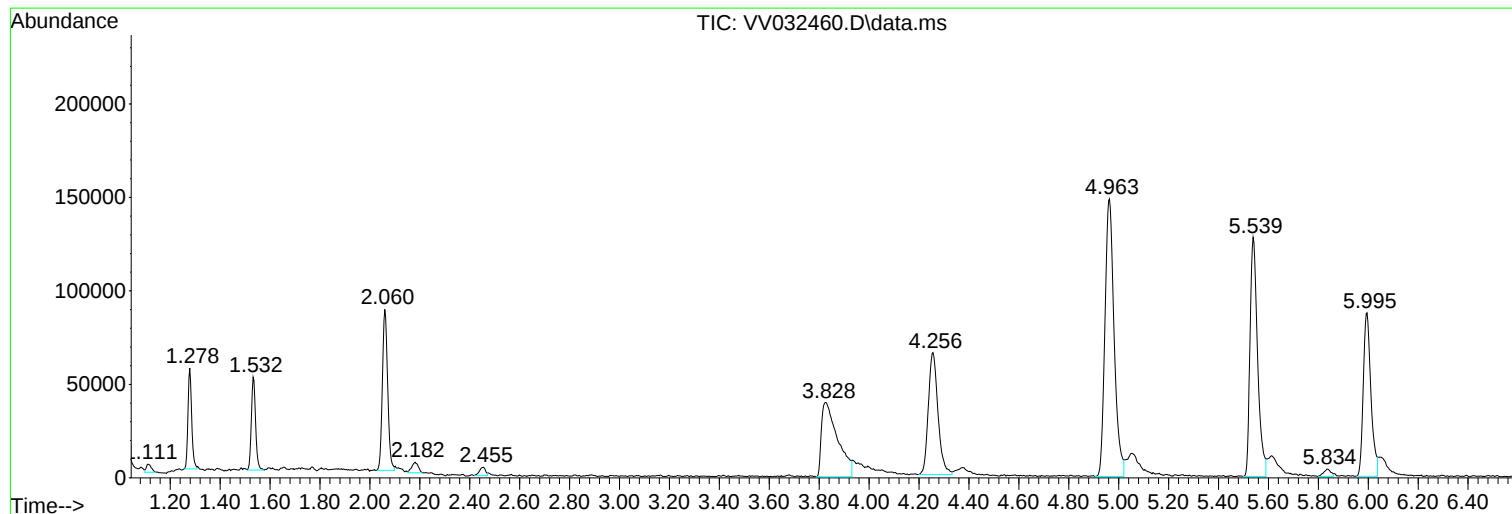

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101823\
Data File : VV032460.D
Acq On : 18 Oct 2023 10:36
Operator : SY/MD
Sample : VV1018WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK372

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101823\
Data File : VV032460.D
Acq On : 18 Oct 2023 10:36
Operator : SY/MD
Sample : VV1018WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK372

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc