

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101823\
 Data File : VV032467.D
 Acq On : 18 Oct 2023 13:31
 Operator : SY/MD
 Sample : 04903-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032467.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	8	14	20	rBV	65355	61318	13.90%	1.527%
2	1.153	31	35	41	rVB	5456	5457	1.24%	0.136%
3	1.191	41	47	53	rBV	22305	21258	4.82%	0.529%
4	1.278	65	74	84	rBV2	91697	104613	23.71%	2.605%
5	1.532	145	153	163	rBV	56720	66828	15.15%	1.664%
6	1.597	166	173	183	rVB2	11477	15523	3.52%	0.387%
7	1.725	206	213	220	rBV3	4393	6668	1.51%	0.166%
8	1.764	220	225	239	rVB2	9154	12415	2.81%	0.309%
9	2.060	306	317	330	rBV	93840	137799	31.24%	3.432%
10	2.185	346	356	367	rVB3	12397	23307	5.28%	0.580%
11	2.696	503	515	525	rBV3	3148	7304	1.66%	0.182%
12	2.969	590	600	612	rVB10	2652	5858	1.33%	0.146%
13	3.802	849	859	895	rBV2	46486	158145	35.85%	3.938%
14	4.252	984	999	1022	rBV	58756	154520	35.03%	3.848%
15	4.368	1025	1035	1055	rVB3	10715	28918	6.56%	0.720%
16	4.587	1091	1103	1106	rBV9	2393	4490	1.02%	0.112%
17	4.960	1203	1219	1236	rBV2	149172	376007	85.24%	9.364%
18	5.535	1386	1398	1415	rBV	113265	240963	54.62%	6.001%
19	5.992	1525	1540	1554	rBV	87075	188877	42.82%	4.704%
20	6.918	1818	1828	1854	rBV2	40082	83498	18.93%	2.079%
21	7.246	1919	1930	1948	rBV	170182	327195	74.17%	8.149%
22	7.323	1949	1954	1972	rVB	15784	31577	7.16%	0.786%
23	7.558	2014	2027	2054	rBV2	23952	50566	11.46%	1.259%
24	7.879	2115	2127	2146	rBV2	14972	32665	7.40%	0.813%
25	8.030	2158	2174	2206	rBV	207445	441139	100.00%	10.986%
26	8.789	2397	2410	2437	rBV	186362	332054	75.27%	8.270%
27	8.953	2451	2461	2475	rBV	16262	28680	6.50%	0.714%
28	9.079	2489	2500	2521	rBV	37431	67264	15.25%	1.675%
29	9.484	2617	2626	2638	rBV2	14989	25184	5.71%	0.627%
30	10.156	2825	2835	2854	rVB2	72815	115274	26.13%	2.871%
31	10.294	2871	2878	2880	rBV3	6482	6810	1.54%	0.170%
32	10.329	2880	2889	2899	rVB	29564	49582	11.24%	1.235%
33	10.390	2899	2908	2914	rBV	14504	25411	5.76%	0.633%
34	10.480	2926	2936	2950	rVB2	7193	13038	2.96%	0.325%
35	10.680	2987	2998	3008	rBV3	8531	14362	3.26%	0.358%
36	10.857	3043	3053	3064	rBV	27724	43613	9.89%	1.086%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101823\
Data File : VV032467.D
Acq On : 18 Oct 2023 13:31
Operator : SY/MD
Sample : 04903-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Title : TRACE VOA SFAM1.0

37	11.188	3145	3156	3175	rBV	200522	318040	72.10%	7.921%
38	11.278	3176	3184	3195	rVB3	8468	14616	3.31%	0.364%
39	11.468	3235	3243	3252	rBV2	10160	19073	4.32%	0.475%
40	11.564	3263	3273	3290	rVB	181969	290104	65.76%	7.225%
41	11.959	3388	3396	3402	rBV4	3793	5577	1.26%	0.139%
42	12.059	3418	3427	3433	rBV6	4339	7866	1.78%	0.196%
43	12.197	3459	3470	3479	rBV2	14189	21923	4.97%	0.546%
44	12.297	3492	3501	3509	rVV8	3982	5908	1.34%	0.147%
45	12.821	3657	3664	3675	rVB5	6703	10126	2.30%	0.252%
46	13.445	3850	3858	3868	rBV2	9034	13988	3.17%	0.348%




Sum of corrected areas: 4015401

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101823\
Data File : VV032467.D
Acq On : 18 Oct 2023 13:31
Operator : SY/MD
Sample : 04903-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

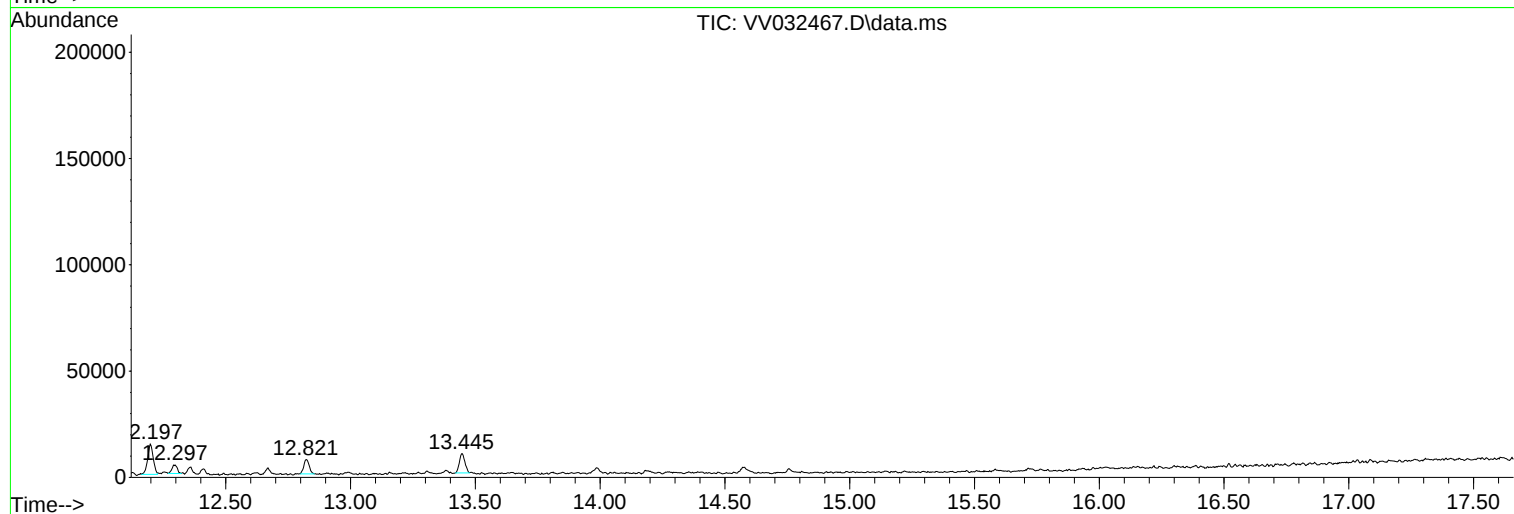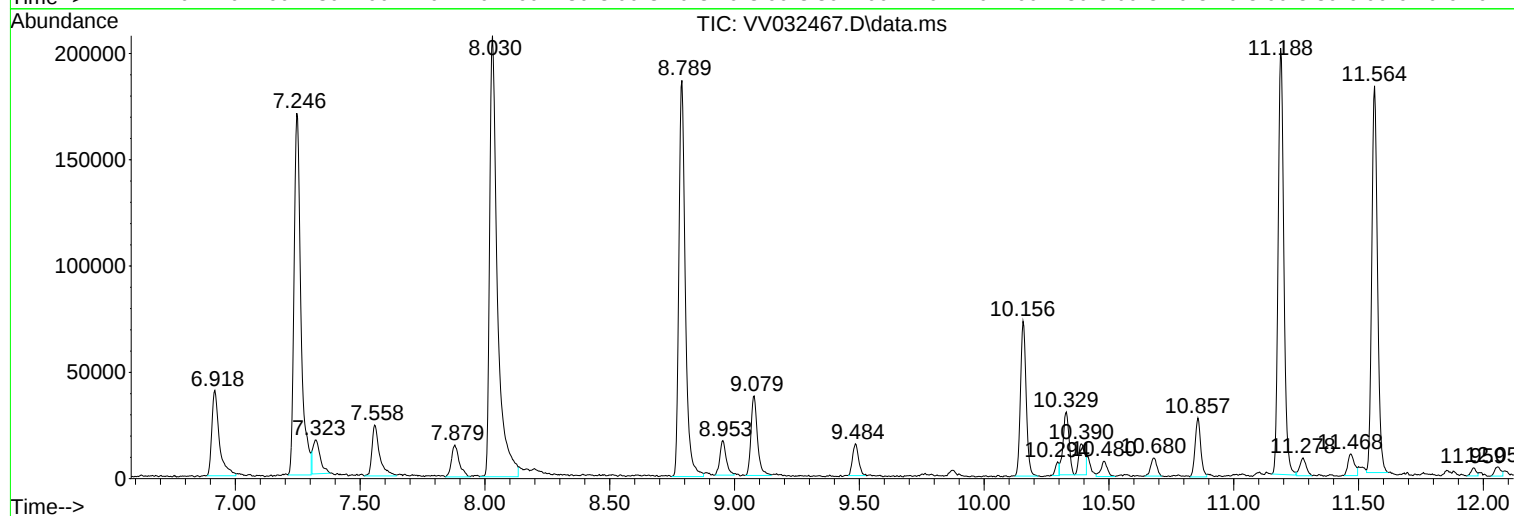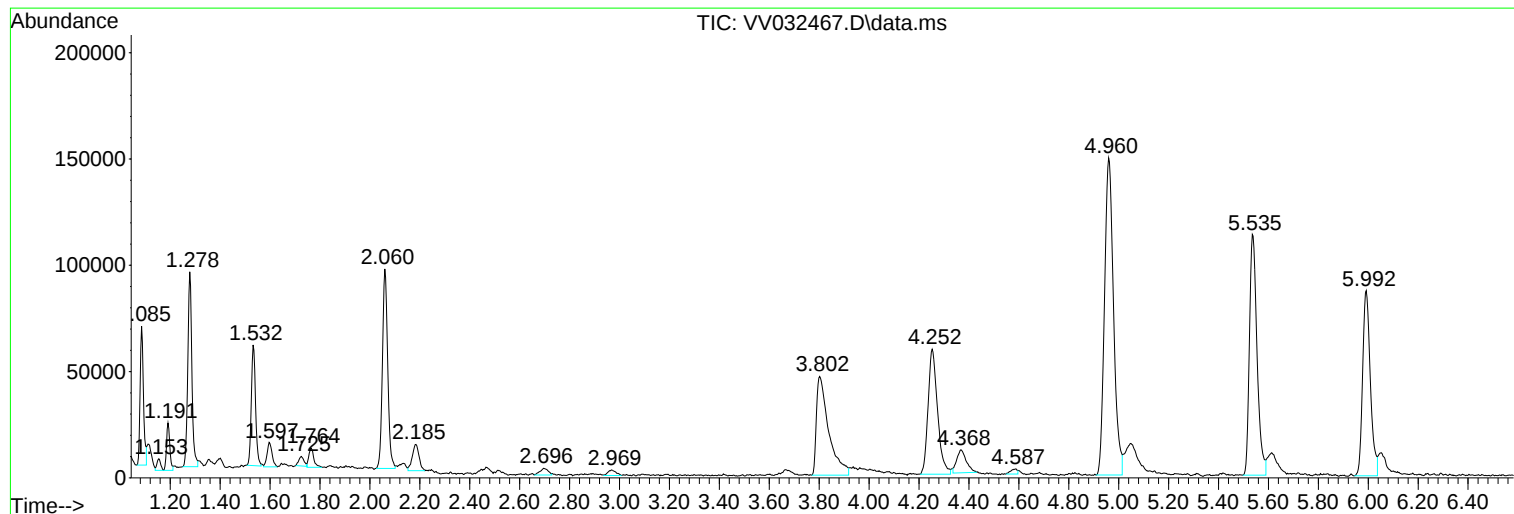

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101823\
Data File : VV032467.D
Acq On : 18 Oct 2023 13:31
Operator : SY/MD
Sample : 04903-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF7










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.085	1.27 ug/L	61318	1,4-Difluorobenzene	5.535

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propene	42	C3H6	000115-07-1	39
2			2-Oxetanone, 4-methyl-	86	C4H6O2	003068-88-0	4
3			Cyclopropane	42	C3H6	000075-19-4	4
4			Cyclopropane	42	C3H6	000075-19-4	4
5			Propane	44	C3H8	000074-98-6	4

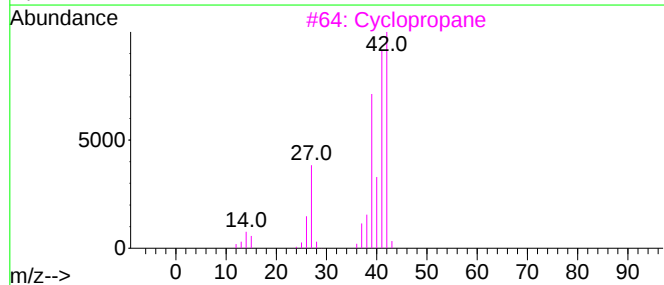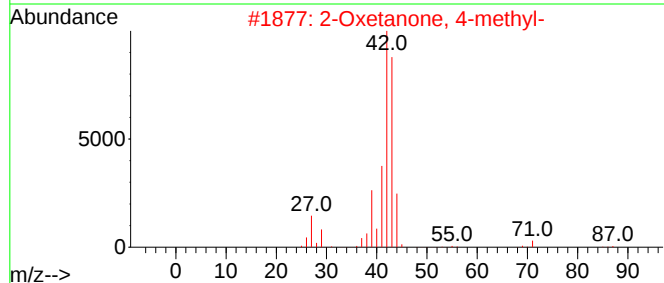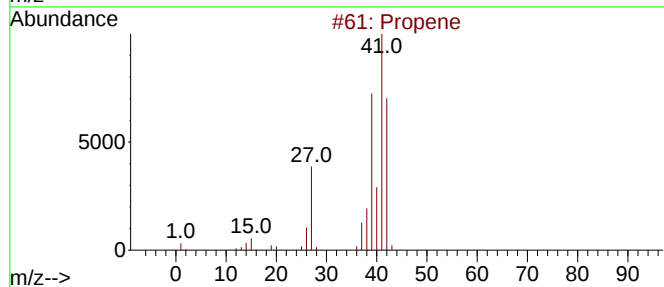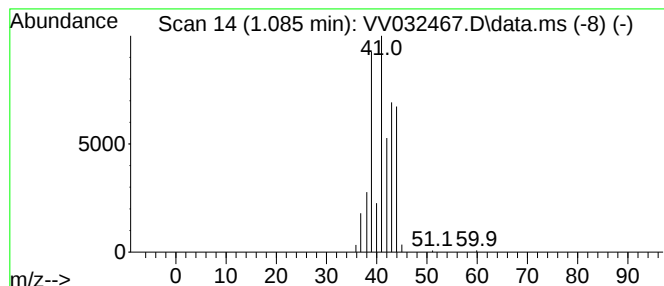

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101823\
Data File : VV032467.D
Acq On : 18 Oct 2023 13:31
Operator : SY/MD
Sample : 04903-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	1.085	1.3	ug/L	61318	1	5.535	240963	5.0