

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101823\
 Data File : VV032471.D
 Acq On : 18 Oct 2023 15:08
 Operator : SY/MD
 Sample : 04918-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AG9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032471.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	9	14	17	rBV2	6367	6197	1.26%	0.158%
2	1.153	30	35	42	rVB	5078	5234	1.06%	0.134%
3	1.278	65	74	85	rBV	76650	82969	16.86%	2.117%
4	1.355	92	98	104	rBV	9088	10567	2.15%	0.270%
5	1.532	145	153	166	rVV	62369	72638	14.76%	1.854%
6	2.060	306	317	331	rBV	99111	148896	30.26%	3.800%
7	2.137	335	341	346	rVV5	5807	9530	1.94%	0.243%
8	2.182	347	355	367	rVV3	15785	31426	6.39%	0.802%
9	2.706	505	518	535	rBV	50863	108965	22.15%	2.781%
10	3.802	849	859	887	rBV	49851	162160	32.96%	4.138%
11	4.252	980	999	1019	rBV2	61827	164416	33.42%	4.196%
12	4.365	1022	1034	1056	rVB4	10707	32176	6.54%	0.821%
13	4.960	1200	1219	1236	rBV2	163277	412944	83.93%	10.538%
14	5.535	1386	1398	1415	rBV	123435	259608	52.76%	6.625%
15	5.992	1526	1540	1554	rBV	96705	203496	41.36%	5.193%
16	6.918	1817	1828	1841	rBV	42826	83285	16.93%	2.125%
17	7.246	1917	1930	1969	rBV	186637	373153	75.84%	9.522%
18	7.558	2018	2027	2041	rBV	26102	51040	10.37%	1.302%
19	7.879	2117	2127	2139	rBV3	8508	16098	3.27%	0.411%
20	8.030	2164	2174	2209	rBV	234482	492019	100.00%	12.555%
21	8.191	2218	2224	2236	rVB	3668	7133	1.45%	0.182%
22	8.786	2398	2409	2436	rBV	202859	360840	73.34%	9.208%
23	9.079	2492	2500	2508	rBV9	3481	6101	1.24%	0.156%
24	10.156	2823	2835	2856	rBV	78894	127437	25.90%	3.252%
25	10.329	2878	2889	2899	rBV2	16393	26483	5.38%	0.676%
26	11.188	3141	3156	3183	rBV	212344	337604	68.62%	8.615%
27	11.564	3261	3273	3293	rVB	192995	308415	62.68%	7.870%
28	12.197	3459	3470	3480	rBV2	6084	10856	2.21%	0.277%
29	12.294	3492	3500	3511	rVB7	4988	7075	1.44%	0.181%




Sum of corrected areas: 3918761

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101823\
Data File : VV032471.D
Acq On : 18 Oct 2023 15:08
Operator : SY/MD
Sample : 04918-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

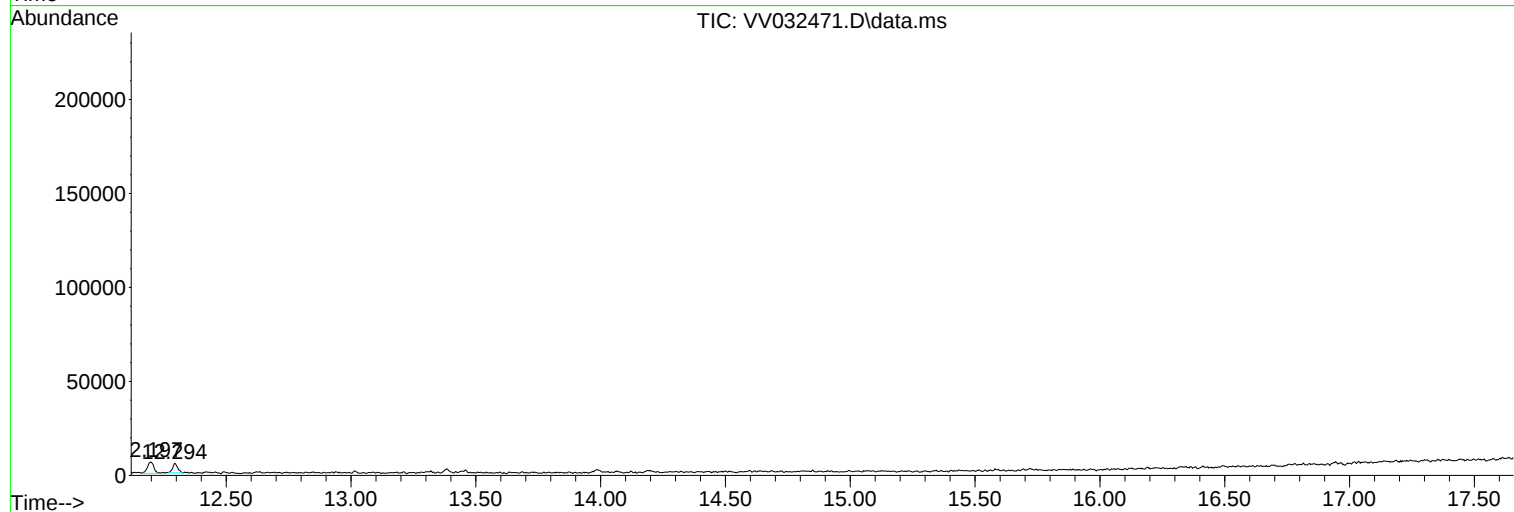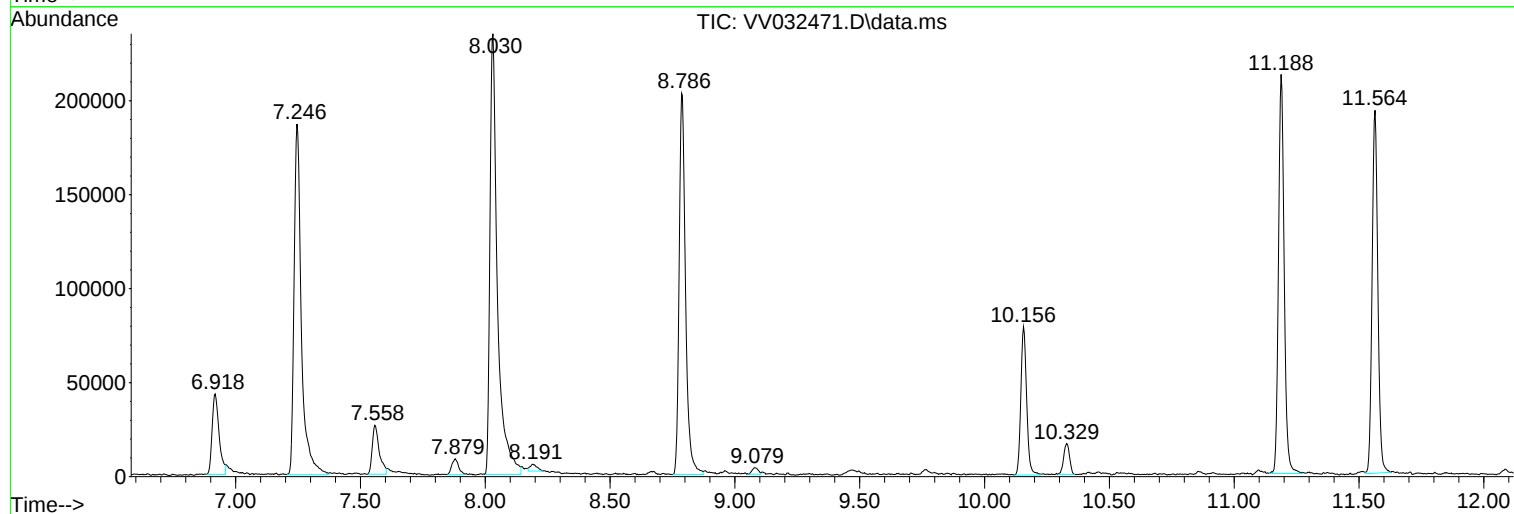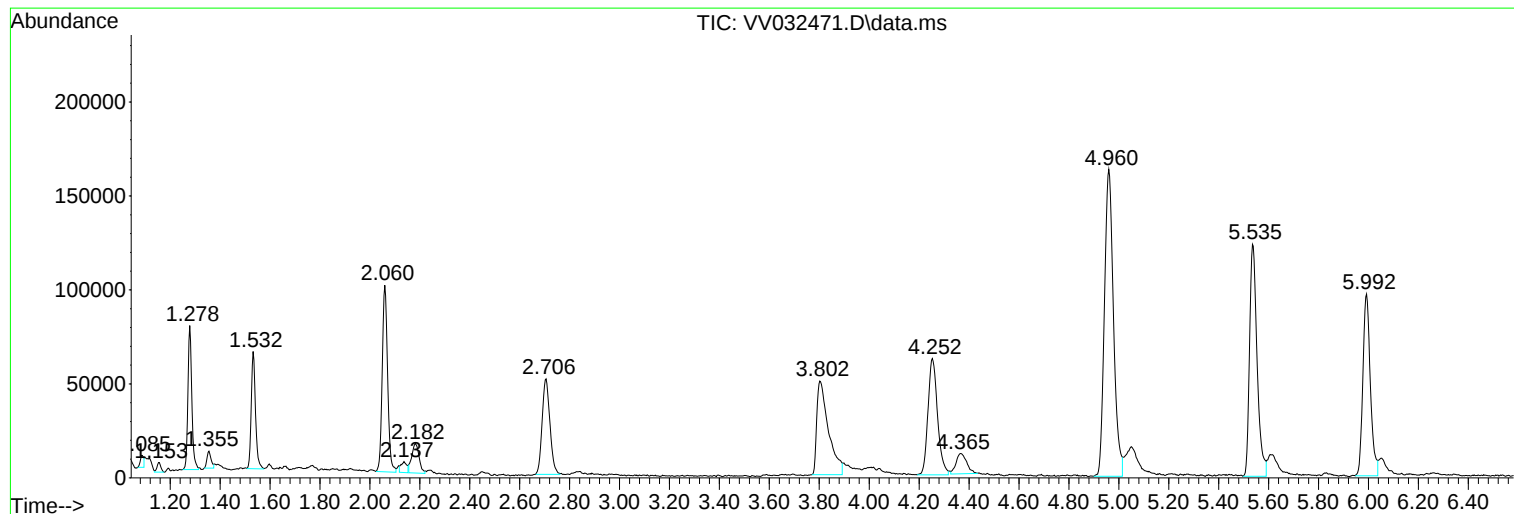

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101823\
Data File : VV032471.D
Acq On : 18 Oct 2023 15:08
Operator : SY/MD
Sample : 04918-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101823\
Data File : VV032471.D
Acq On : 18 Oct 2023 15:08
Operator : SY/MD
Sample : 04918-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
