

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101823\
 Data File : VV032473.D
 Acq On : 18 Oct 2023 15:57
 Operator : SY/MD
 Sample : 04944-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4968

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032473.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.117	12	24	31	rVB2	5272	10663	2.59%	0.324%
2	1.217	49	55	65	rBV2	6445	8941	2.18%	0.271%
3	1.278	66	74	85	rVV	63869	68722	16.72%	2.085%
4	1.532	145	153	169	rVB	54726	64512	15.70%	1.957%
5	2.060	306	317	331	rBV	83381	122226	29.74%	3.709%
6	2.182	345	355	369	rVB2	13161	27937	6.80%	0.848%
7	3.805	847	860	898	rBV2	49648	177424	43.18%	5.383%
8	4.256	982	1000	1018	rBV2	53699	145314	35.36%	4.409%
9	4.368	1024	1035	1050	rVB	8773	21180	5.15%	0.643%
10	4.960	1203	1219	1238	rBV2	139862	358970	87.36%	10.892%
11	5.535	1384	1398	1417	rBV	111311	238798	58.11%	7.246%
12	5.838	1487	1492	1506	rVB	2452	4698	1.14%	0.143%
13	5.992	1525	1540	1555	rBV2	81198	176757	43.01%	5.363%
14	6.918	1817	1828	1853	rBV	37839	78832	19.18%	2.392%
15	7.246	1919	1930	1949	rBV	157310	302947	73.72%	9.192%
16	7.561	2018	2028	2041	rBV	21843	43666	10.63%	1.325%
17	8.030	2164	2174	2215	rBV	189611	410924	100.00%	12.468%
18	8.789	2395	2410	2433	rBV	184042	328812	80.02%	9.977%
19	9.082	2492	2501	2516	rVB2	8273	14279	3.47%	0.433%
20	9.487	2616	2627	2634	rBV6	3596	5933	1.44%	0.180%
21	10.156	2824	2835	2857	rVB	63627	106245	25.86%	3.224%
22	10.329	2879	2889	2896	rVB3	5650	8641	2.10%	0.262%
23	10.863	3046	3055	3064	rBV5	3911	6323	1.54%	0.192%
24	11.188	3146	3156	3173	rBV	191153	301023	73.26%	9.134%
25	11.564	3262	3273	3289	rVV	161349	257442	62.65%	7.811%
26	12.194	3464	3469	3479	rVB4	2947	4527	1.10%	0.137%




Sum of corrected areas: 3295736

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101823\
Data File : VV032473.D
Acq On : 18 Oct 2023 15:57
Operator : SY/MD
Sample : 04944-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4968

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

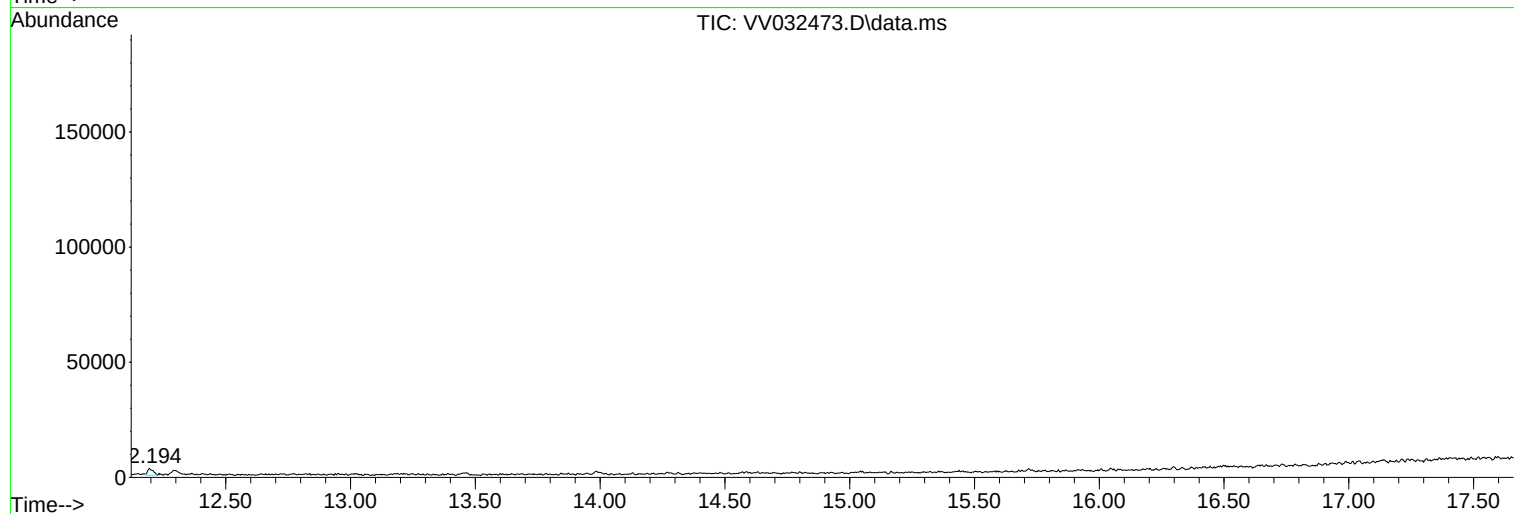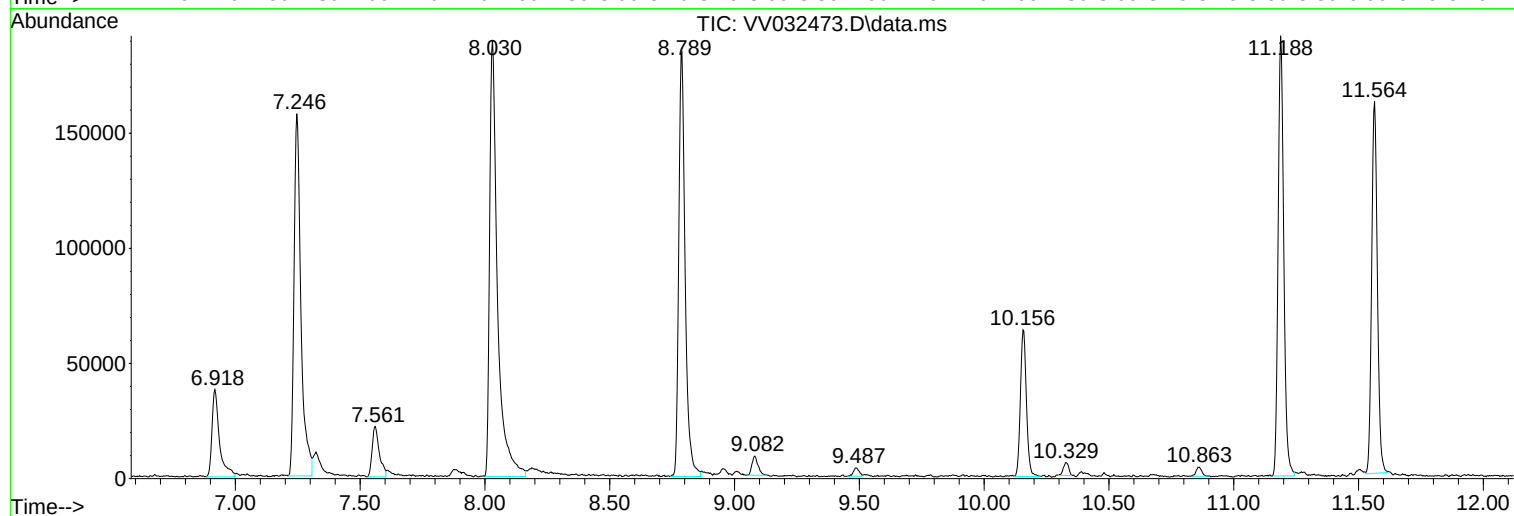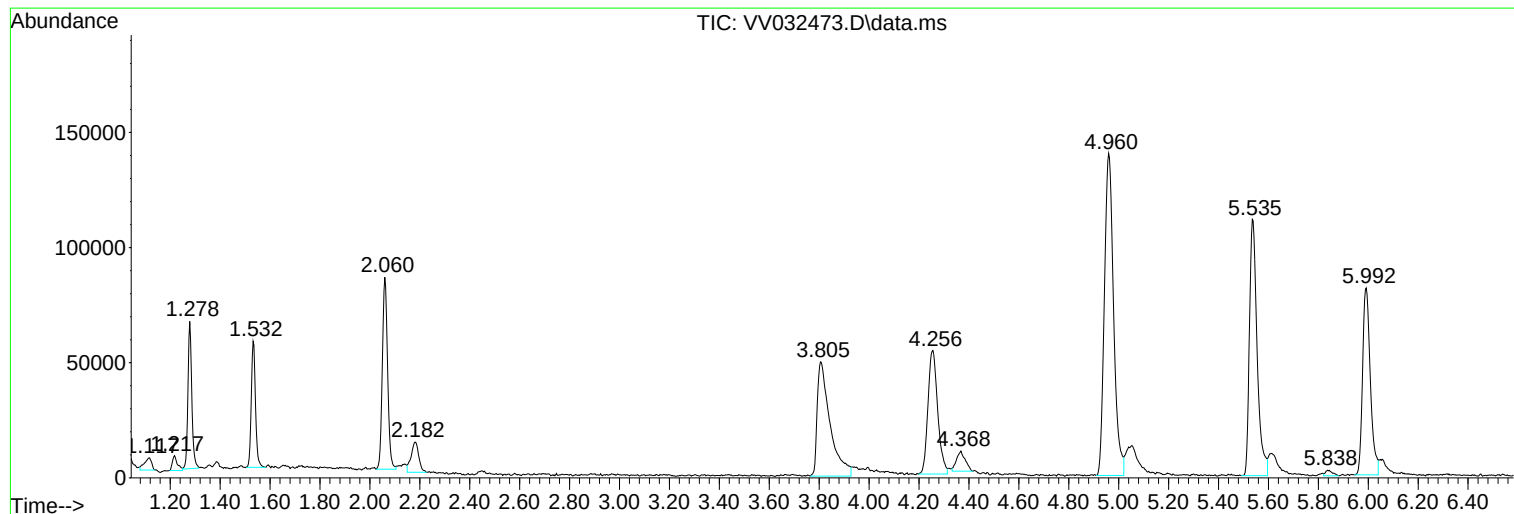

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101823\
Data File : VV032473.D
Acq On : 18 Oct 2023 15:57
Operator : SY/MD
Sample : 04944-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4968

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101823\
Data File : VV032473.D
Acq On : 18 Oct 2023 15:57
Operator : SY/MD
Sample : 04944-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4968

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc