

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101823\
 Data File : VV032476.D
 Acq On : 18 Oct 2023 17:09
 Operator : SY/MD
 Sample : 04944-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49T0

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032476.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.111	17	22	34	rVB2	6570	10933	2.74%	0.342%
2	1.278	67	74	88	rBV	61818	65042	16.30%	2.037%
3	1.384	102	107	115	rVB	5358	6724	1.69%	0.211%
4	1.532	145	153	165	rBV	53395	61796	15.49%	1.935%
5	2.060	307	317	330	rVV	80555	117448	29.44%	3.677%
6	2.182	347	355	371	rVB	12779	25843	6.48%	0.809%
7	3.806	849	860	896	rBV3	53101	187929	47.10%	5.884%
8	4.252	982	999	1020	rBV2	54632	147465	36.96%	4.617%
9	4.362	1022	1033	1034	rBV6	6740	8052	2.02%	0.252%
10	4.960	1201	1219	1237	rBV2	137873	352916	88.45%	11.050%
11	5.539	1387	1399	1416	rBV	106337	228912	57.37%	7.168%
12	5.992	1525	1540	1554	rBV	82919	176394	44.21%	5.523%
13	6.918	1815	1828	1853	rBV	35433	76654	19.21%	2.400%
14	7.246	1920	1930	1950	rBV	150610	291712	73.11%	9.134%
15	7.558	2017	2027	2048	rBV	21771	45746	11.47%	1.432%
16	8.030	2161	2174	2205	rBV	190395	398999	100.00%	12.493%
17	8.789	2399	2410	2435	rBV	177069	311540	78.08%	9.755%
18	9.082	2493	2501	2513	rBV5	5440	9918	2.49%	0.311%
19	9.490	2620	2628	2634	rBV7	2343	4009	1.00%	0.126%
20	10.156	2826	2835	2851	rBV	65301	105958	26.56%	3.318%
21	11.188	3146	3156	3176	rBV	182921	287683	72.10%	9.008%
22	11.497	3239	3252	3259	rBV8	5831	12241	3.07%	0.383%
23	11.564	3262	3273	3292	rVB	161125	259789	65.11%	8.134%




Sum of corrected areas: 3193703

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101823\
Data File : VV032476.D
Acq On : 18 Oct 2023 17:09
Operator : SY/MD
Sample : 04944-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49T0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

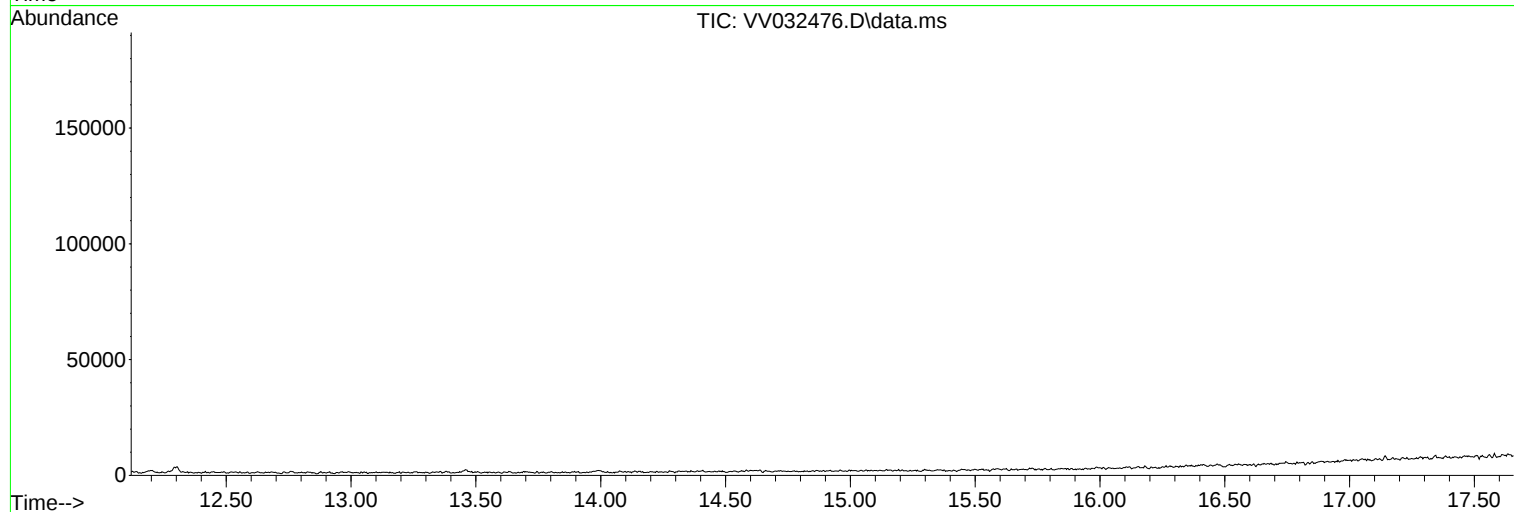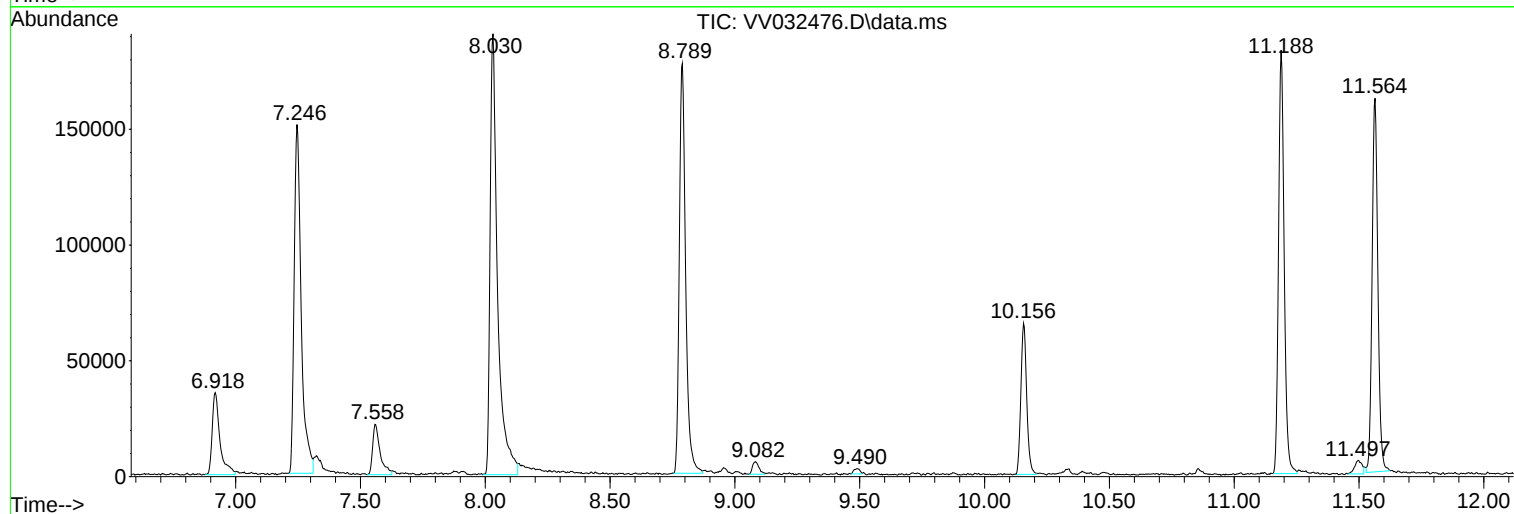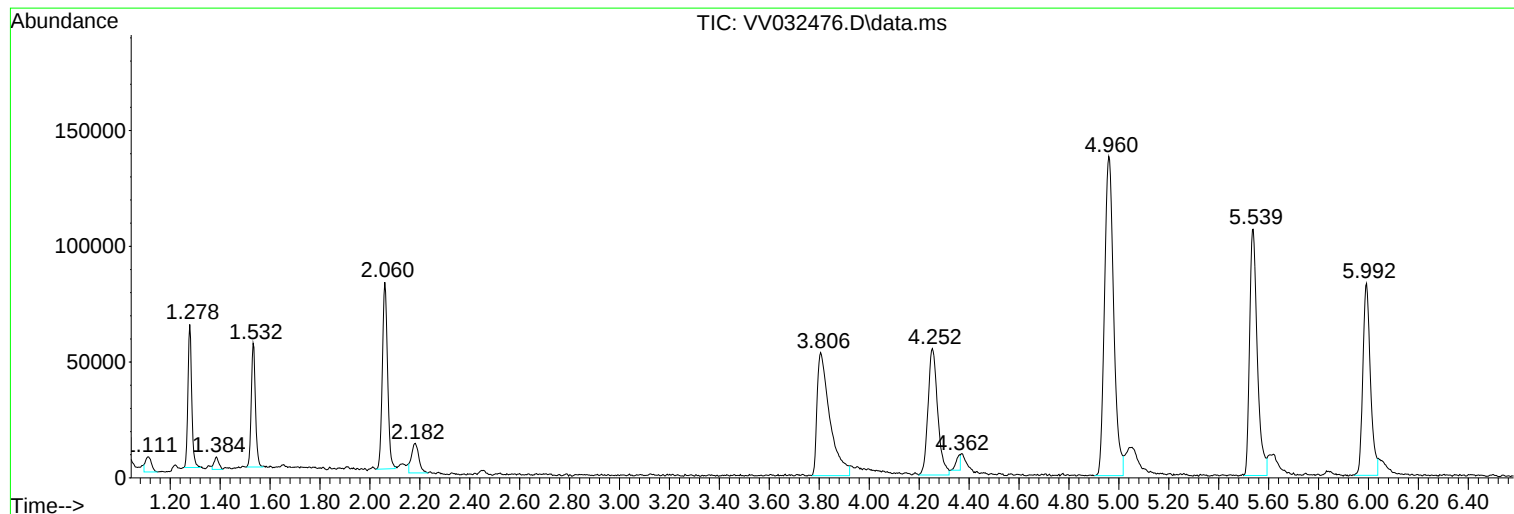

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101823\
Data File : VV032476.D
Acq On : 18 Oct 2023 17:09
Operator : SY/MD
Sample : 04944-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49T0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101823\
Data File : VV032476.D
Acq On : 18 Oct 2023 17:09
Operator : SY/MD
Sample : 04944-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49T0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------