

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101823\
 Data File : VV032478.D
 Acq On : 18 Oct 2023 17:57
 Operator : SY/MD
 Sample : 04944-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49F3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032478.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.114	16	23	32	rVB2	6651	10995	2.81%	0.353%
2	1.278	67	74	89	rVB	59497	63734	16.29%	2.049%
3	1.532	143	153	163	rBV	53250	63270	16.17%	2.034%
4	2.060	307	317	330	rBV	79141	114261	29.20%	3.673%
5	2.182	344	355	368	rVB2	12476	26244	6.71%	0.844%
6	3.806	849	860	891	rBV	42239	143636	36.70%	4.618%
7	4.253	981	999	1021	rBV	53582	145359	37.15%	4.673%
8	4.368	1023	1035	1054	rVB5	8150	24565	6.28%	0.790%
9	4.960	1204	1219	1238	rBV2	134822	342855	87.61%	11.022%
10	5.535	1387	1398	1416	rBV	106015	226575	57.90%	7.284%
11	5.609	1418	1421	1440	rVB2	9161	18562	4.74%	0.597%
12	5.992	1526	1540	1555	rBV	81370	173194	44.26%	5.568%
13	6.053	1557	1559	1566	rVB5	4480	4518	1.15%	0.145%
14	6.918	1817	1828	1855	rBV	36456	77051	19.69%	2.477%
15	7.246	1918	1930	1951	rBV	149054	289292	73.93%	9.300%
16	7.561	2013	2028	2049	rBV	20660	44705	11.42%	1.437%
17	8.031	2164	2174	2213	rBV	179702	391328	100.00%	12.580%
18	8.789	2399	2410	2438	rBV	172601	312490	79.85%	10.046%
19	9.082	2495	2501	2512	rBV6	3181	5021	1.28%	0.161%
20	10.156	2822	2835	2849	rBV2	63441	102498	26.19%	3.295%
21	11.188	3146	3156	3173	rBV	179629	284606	72.73%	9.149%
22	11.564	3261	3273	3288	rVV	155139	245873	62.83%	7.904%




Sum of corrected areas: 3110632

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101823\
Data File : VV032478.D
Acq On : 18 Oct 2023 17:57
Operator : SY/MD
Sample : 04944-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49F3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

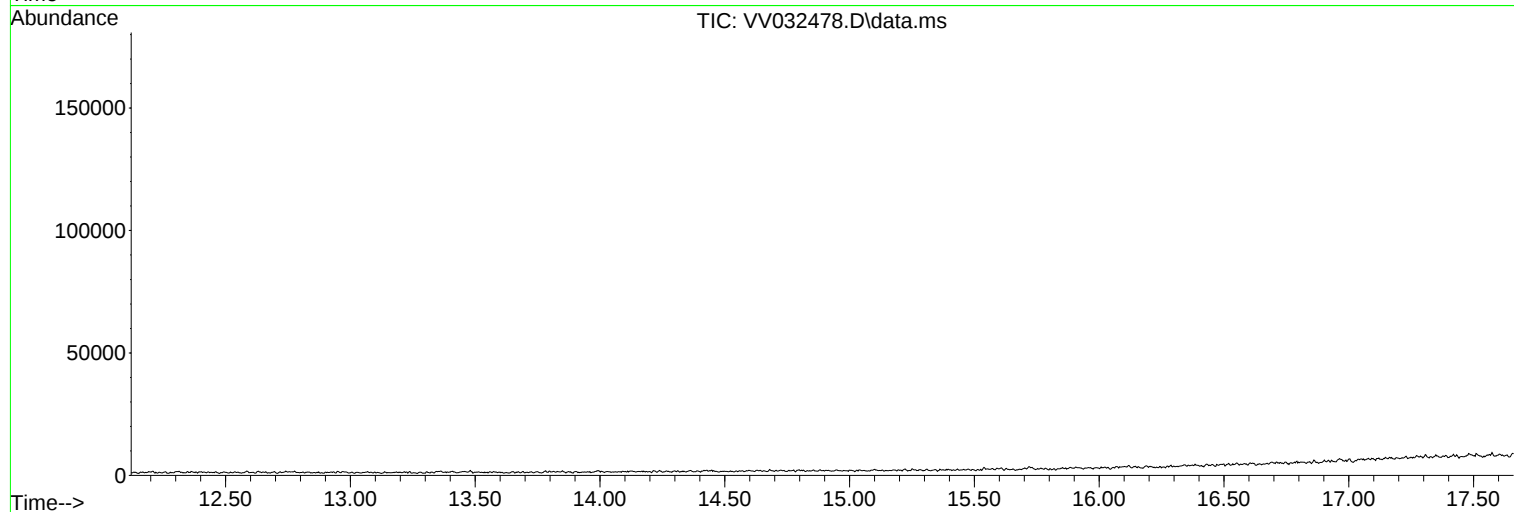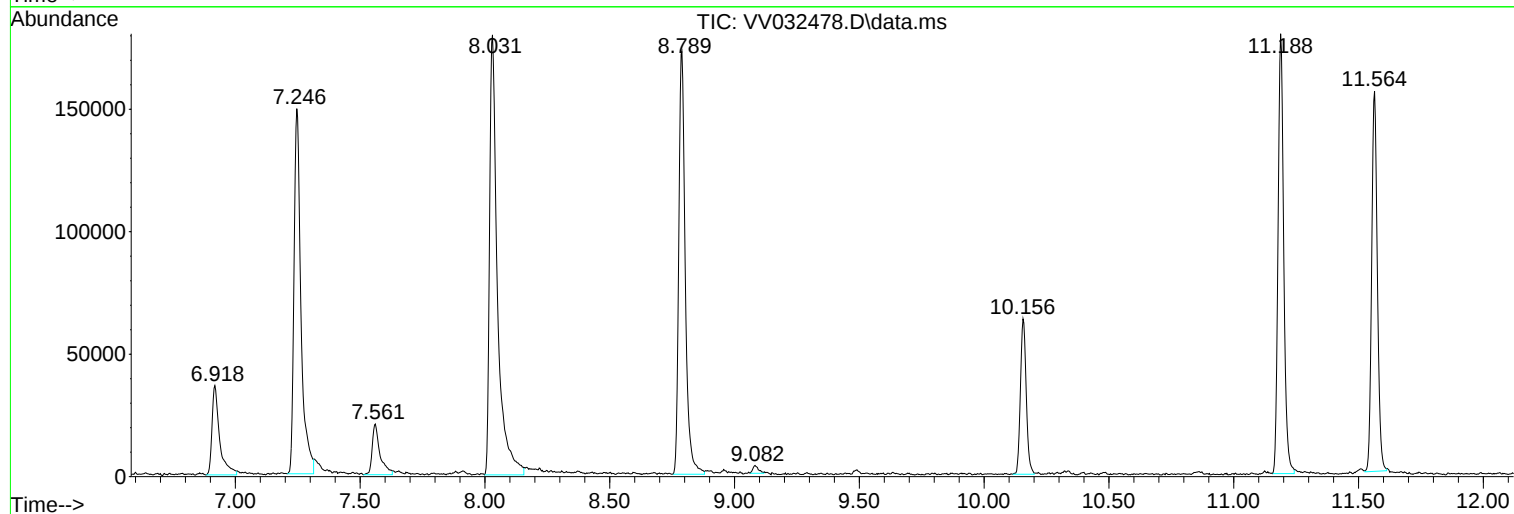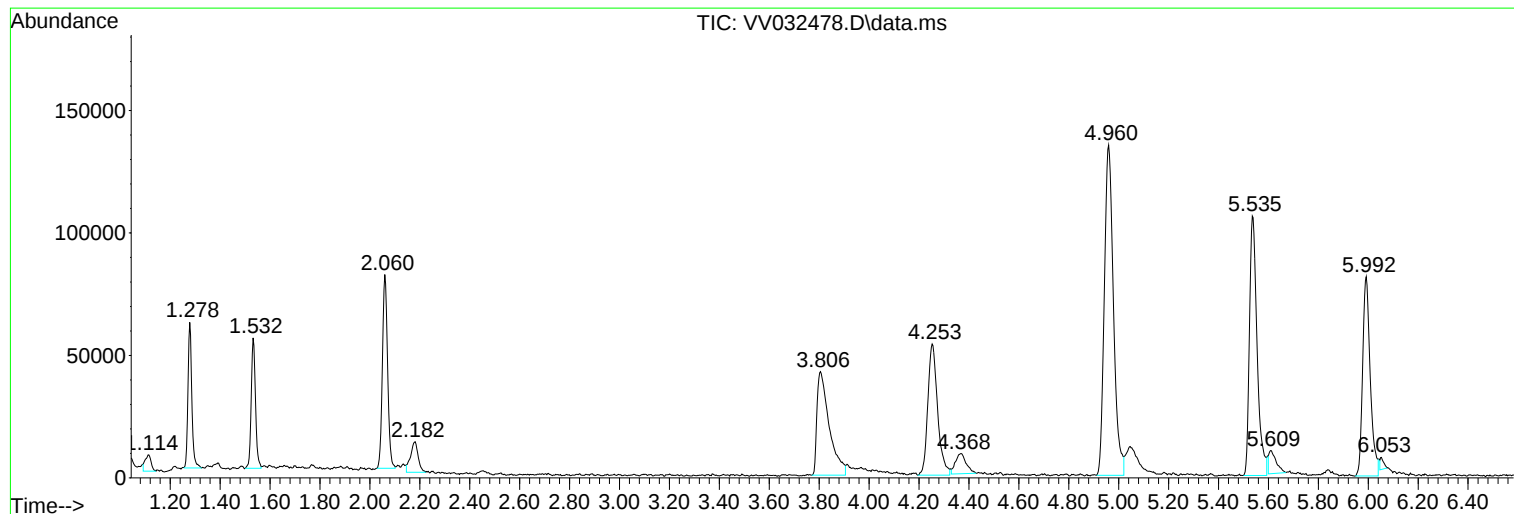

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101823\
Data File : VV032478.D
Acq On : 18 Oct 2023 17:57
Operator : SY/MD
Sample : 04944-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49F3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101823\
Data File : VV032478.D
Acq On : 18 Oct 2023 17:57
Operator : SY/MD
Sample : 04944-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49F3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------