

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101823\
 Data File : VV032479.D
 Acq On : 18 Oct 2023 18:22
 Operator : SY/MD
 Sample : 04944-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49F4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032479.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.111	15	22	29	rVB2	6487	10199	2.73%	0.336%
2	1.278	66	74	86	rBV	58977	63135	16.91%	2.083%
3	1.532	146	153	163	rBV	49638	57846	15.49%	1.908%
4	2.060	307	317	332	rBV	78762	117838	31.56%	3.888%
5	2.175	345	353	366	rVB2	11420	24216	6.49%	0.799%
6	3.809	850	861	887	rBV	40422	137043	36.71%	4.521%
7	4.252	984	999	1020	rBV2	53049	141252	37.83%	4.660%
8	4.368	1023	1035	1042	rBV3	6083	13596	3.64%	0.449%
9	4.960	1202	1219	1239	rBV2	132263	343541	92.02%	11.334%
10	5.539	1387	1399	1413	rBV	105715	220021	58.93%	7.259%
11	5.844	1482	1494	1500	rBV10	2281	4014	1.08%	0.132%
12	5.992	1527	1540	1557	rBV2	79701	172098	46.10%	5.678%
13	6.918	1818	1828	1853	rBV3	34178	73033	19.56%	2.409%
14	7.246	1919	1930	1950	rBV	147277	283244	75.87%	9.345%
15	7.561	2019	2028	2048	rBV	19768	41877	11.22%	1.382%
16	8.030	2164	2174	2207	rBV2	174028	373339	100.00%	12.317%
17	8.789	2398	2410	2430	rBV	177269	316015	84.65%	10.426%
18	9.085	2490	2502	2510	rBV10	3813	7265	1.95%	0.240%
19	10.156	2823	2835	2850	rBV	62368	101321	27.14%	3.343%
20	11.188	3143	3156	3174	rBV	180355	285805	76.55%	9.429%
21	11.564	3262	3273	3292	rBV	151730	244357	65.45%	8.062%




Sum of corrected areas: 3031055

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101823\
Data File : VV032479.D
Acq On : 18 Oct 2023 18:22
Operator : SY/MD
Sample : 04944-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49F4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

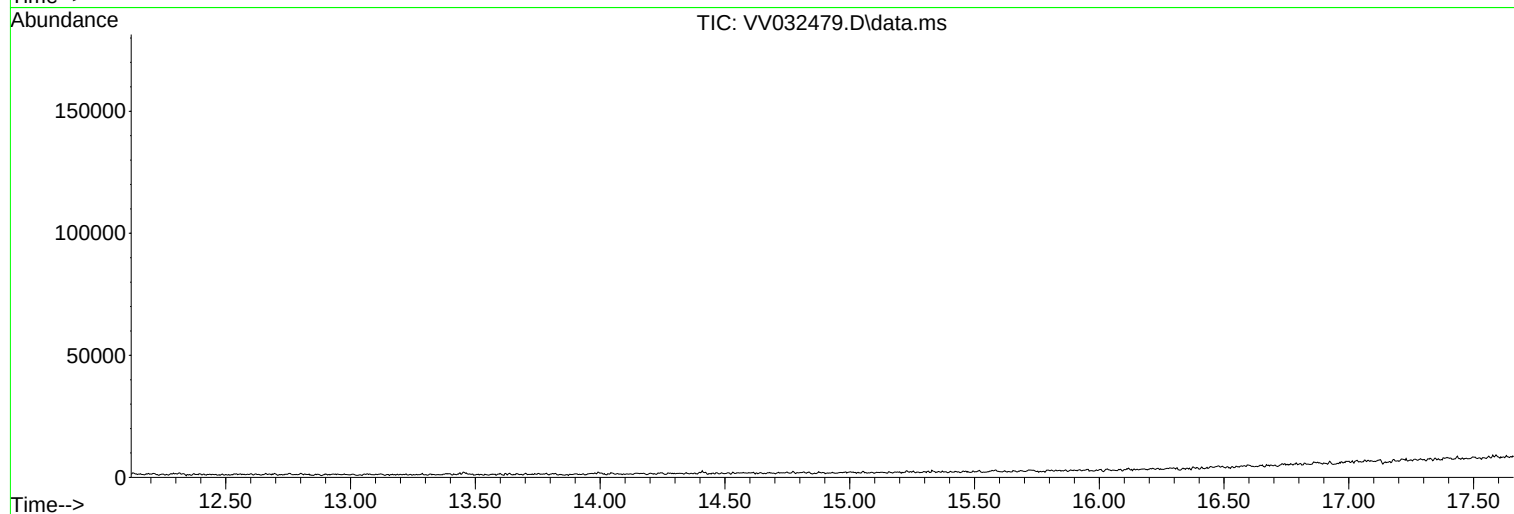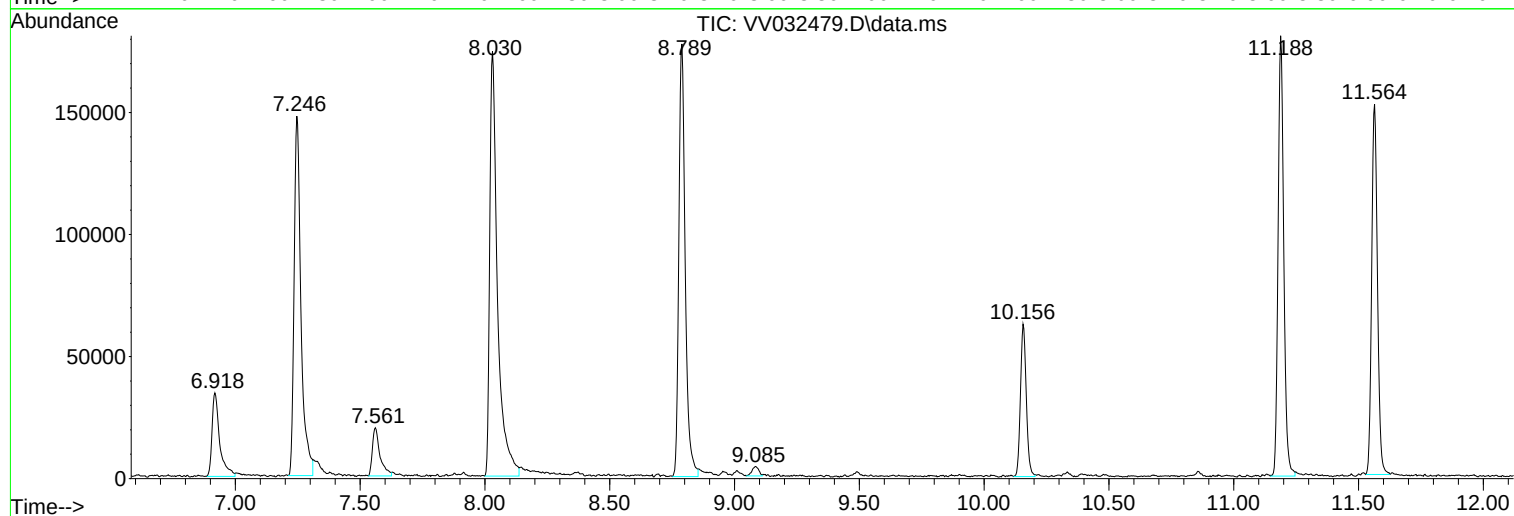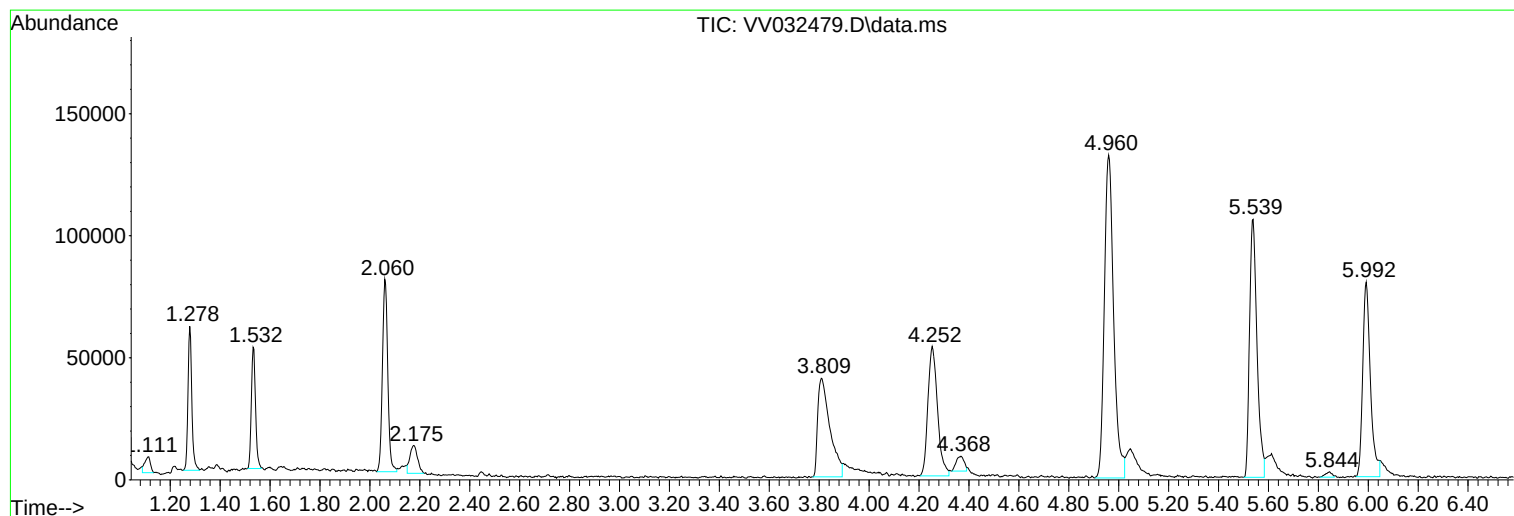

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101823\
Data File : VV032479.D
Acq On : 18 Oct 2023 18:22
Operator : SY/MD
Sample : 04944-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49F4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101823\
Data File : VV032479.D
Acq On : 18 Oct 2023 18:22
Operator : SY/MD
Sample : 04944-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49F4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc