

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101823\
 Data File : VV032481.D
 Acq On : 18 Oct 2023 19:10
 Operator : SY/MD
 Sample : 04944-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49N4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032481.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.214	49	54	63	rBV	7264	8914	2.33%	0.271%
2	1.278	66	74	92	rVB	62648	67490	17.64%	2.048%
3	1.532	145	153	168	rBV	51721	61749	16.14%	1.874%
4	2.060	308	317	333	rBV	92202	134829	35.23%	4.092%
5	3.806	846	860	891	rBV	43020	147904	38.65%	4.489%
6	4.253	979	999	1031	rBV2	61741	168671	44.08%	5.119%
7	4.960	1201	1219	1247	rBV3	141370	376355	98.35%	11.422%
8	5.535	1382	1398	1422	rBV	114963	248701	64.99%	7.548%
9	5.992	1524	1540	1557	rBV2	84618	182846	47.78%	5.549%
10	6.918	1817	1828	1844	rBV	35397	70751	18.49%	2.147%
11	7.246	1918	1930	1946	rBV	159575	291309	76.13%	8.841%
12	7.323	1946	1954	1970	rVB	21066	43467	11.36%	1.319%
13	7.561	2018	2028	2048	rBV2	21840	43943	11.48%	1.334%
14	8.031	2164	2174	2209	rBV	186001	382662	100.00%	11.614%
15	8.786	2395	2409	2434	rBV	183901	317628	83.00%	9.640%
16	8.957	2454	2462	2473	rVB2	5656	9815	2.56%	0.298%
17	9.079	2491	2500	2515	rBV	17297	30639	8.01%	0.930%
18	9.484	2615	2626	2635	rBV3	8168	13548	3.54%	0.411%
19	10.156	2822	2835	2851	rBV	63397	103587	27.07%	3.144%
20	10.391	2898	2908	2915	rBV8	4875	8689	2.27%	0.264%
21	10.860	3046	3054	3062	rBV2	7726	11166	2.92%	0.339%
22	11.188	3145	3156	3172	rBV	184174	292184	76.36%	8.868%
23	11.497	3238	3252	3262	rBV9	7981	19374	5.06%	0.588%
24	11.564	3262	3273	3292	rVB	159162	258653	67.59%	7.850%




Sum of corrected areas: 3294874

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101823\
Data File : VV032481.D
Acq On : 18 Oct 2023 19:10
Operator : SY/MD
Sample : 04944-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49N4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

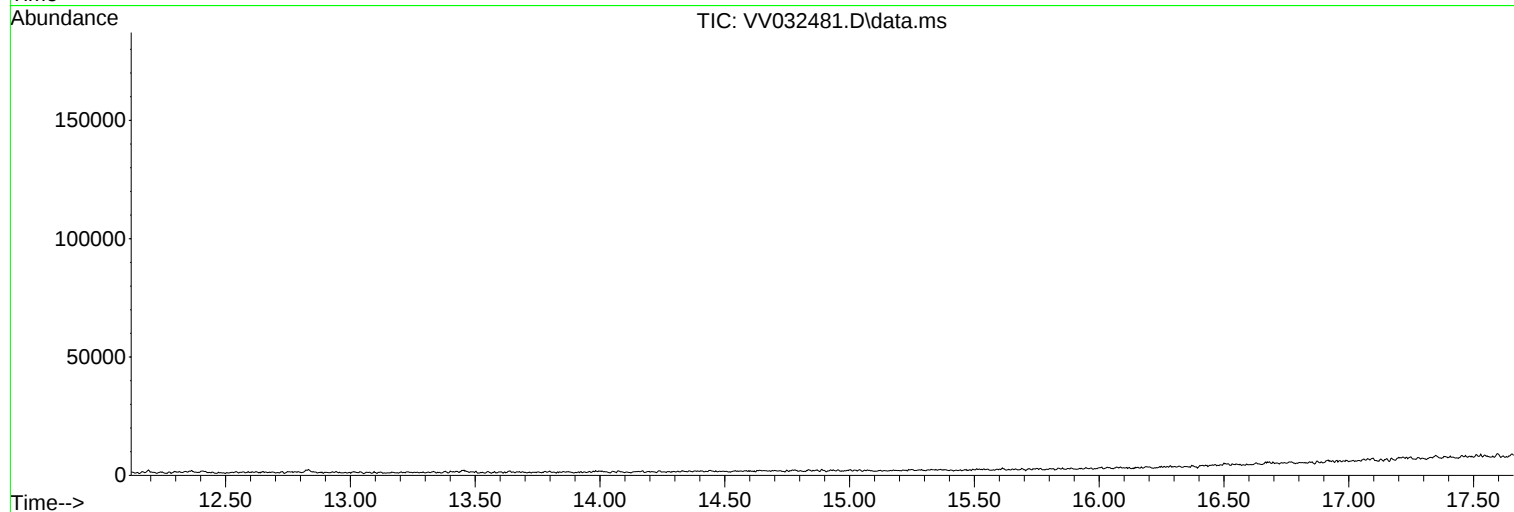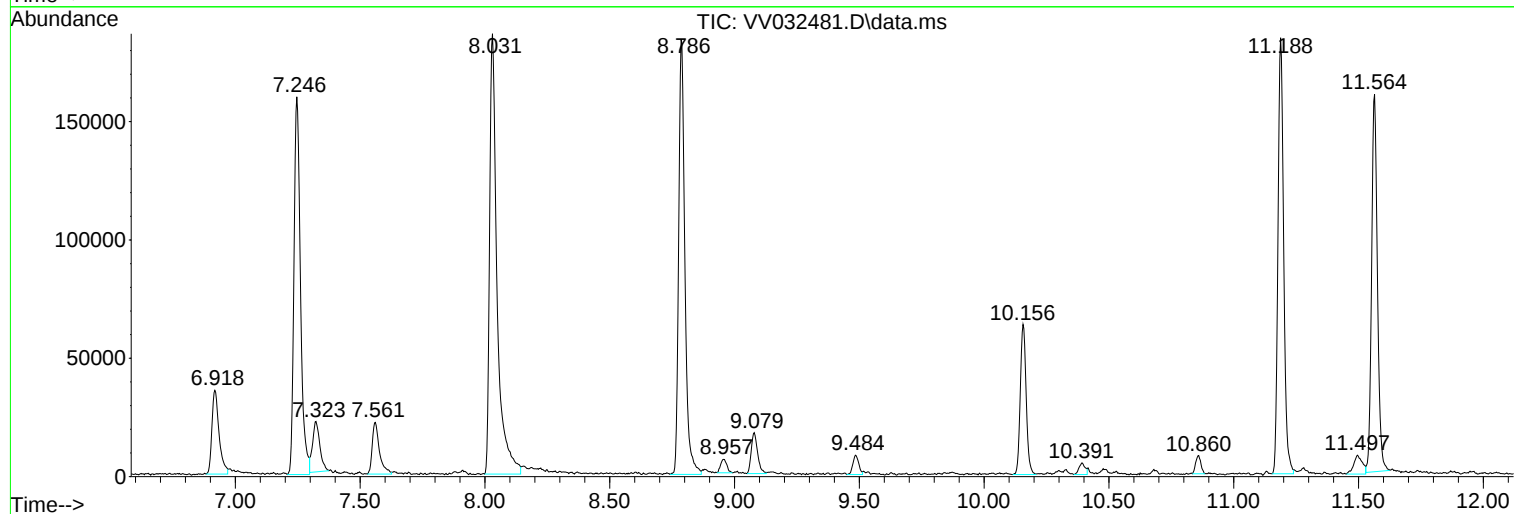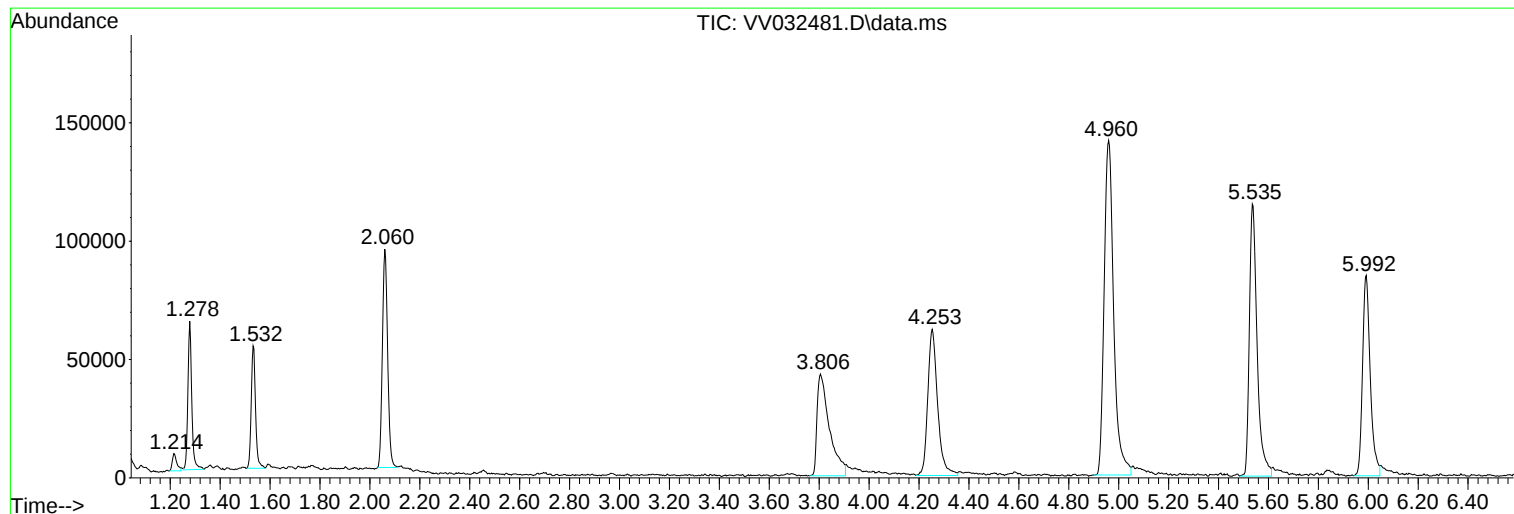

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101823\
Data File : VV032481.D
Acq On : 18 Oct 2023 19:10
Operator : SY/MD
Sample : 04944-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49N4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101823\
Data File : VV032481.D
Acq On : 18 Oct 2023 19:10
Operator : SY/MD
Sample : 04944-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49N4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc