


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101823\
Data File : VV032458.D
Acq On : 18 Oct 2023 08:42
Operator : SY/MD
Sample : BFB222
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB222

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Oct 20 06:17:42 2023

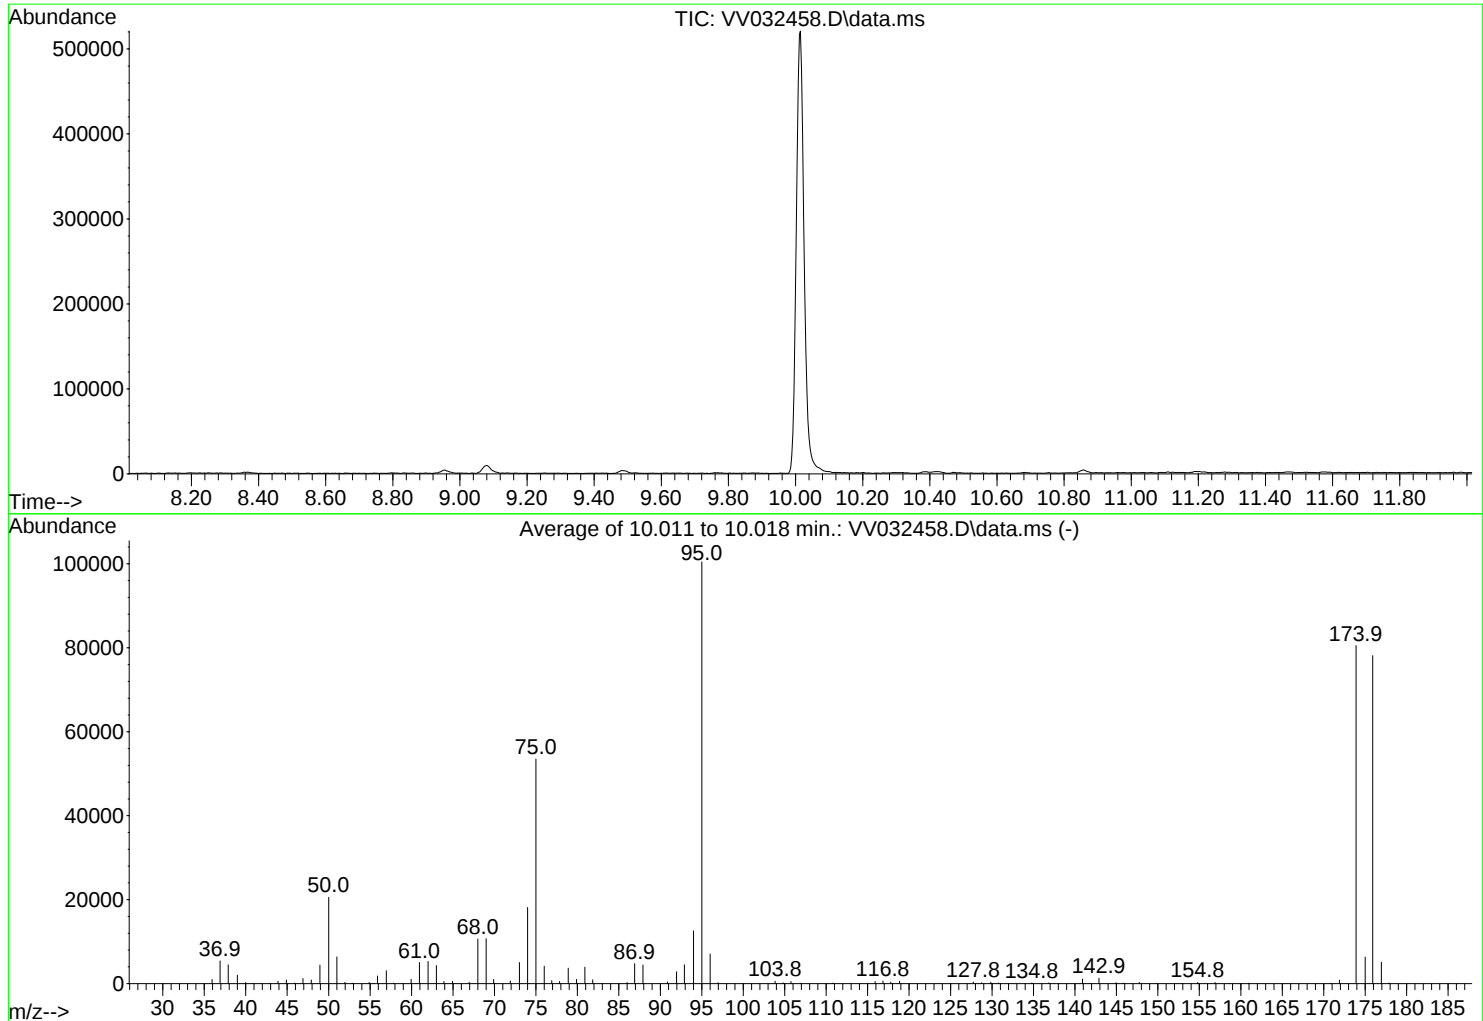

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	20552	PASS
75	95	30	80	53.3	53509	PASS
95	95	100	100	100.0	100469	PASS
96	95	5	9	7.0	7047	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	80.2	80536	PASS
175	174	5	9	7.9	6335	PASS
176	174	95	105	97.0	78136	PASS
177	176	5	10	6.5	5099	PASS

m/z	Abundance
39.70	230.0
43.90	386.0

Instrument :
MSVOA_V
ClientSampleId :
BFB222

m/z	Abundance
35.90	1080.0
36.90	5756.0
37.90	4948.0
39.00	2111.0
40.00	291.0
40.80	156.0
41.80	107.0
42.90	133.0
43.90	1001.0
44.90	904.0
45.90	153.0
46.90	1315.0
47.90	894.0
49.00	4657.0
50.00	21384.0
51.00	6792.0
51.90	317.0
52.80	144.0
54.90	293.0
55.90	1891.0
56.90	3314.0
57.90	133.0
59.90	1031.0
60.90	5102.0
62.00	5560.0
63.00	4650.0
63.90	512.0
64.90	617.0
66.90	399.0
68.00	11100.0
69.00	10860.0
69.90	1008.0
71.90	617.0
73.00	5293.0
74.00	18808.0
75.00	55736.0
76.00	4590.0
76.90	808.0
77.80	476.0
78.90	3880.0
79.90	1003.0
80.90	4047.0
81.90	898.0
82.70	110.0
86.00	287.0
86.90	4976.0
87.90	4536.0
90.90	448.0
91.90	2951.0
92.90	4615.0
94.00	13131.0
95.00	103440.0
96.00	7469.0
97.00	276.0
103.90	574.0
104.80	186.0
105.80	526.0
107.00	120.0
110.80	196.0
113.00	124.0
115.00	119.0
115.90	520.0
116.80	679.0
117.80	393.0
118.90	575.0
123.70	101.0
127.80	365.0
128.70	223.0
129.90	337.0
130.90	183.0
134.80	194.0
136.90	189.0
140.90	1071.0
141.80	139.0
142.90	1257.0
145.00	281.0
145.80	186.0
147.80	303.0
149.80	141.0
154.80	308.0
156.90	257.0
160.90	141.0
170.80	120.0
171.90	838.0
173.90	79952.0
175.00	6530.0
175.90	77472.0
177.00	5281.0
177.90	141.0

Instrument :
MSVOA_V
ClientSampleId :
BFB222

m/z	Abundance
35.90	997.0
36.90	5594.0
37.90	4587.0
39.00	2052.0
40.00	268.0
40.80	127.0
43.00	105.0
43.90	974.0
44.90	897.0
45.90	178.0
46.90	1246.0
47.90	928.0
49.00	4539.0
50.00	21200.0
51.00	6564.0
52.00	313.0
52.80	140.0
54.90	303.0
55.90	1918.0
57.00	3168.0
57.80	151.0
60.00	1029.0
61.00	5133.0
62.00	5454.0
63.00	4447.0
63.90	500.0
64.90	602.0
66.90	361.0
68.00	11052.0
69.00	10954.0
69.90	1066.0
71.90	666.0
73.00	5213.0
74.00	18696.0
75.00	55328.0
76.00	4278.0
76.90	759.0
77.90	500.0
78.90	3743.0
79.90	1031.0
80.90	4070.0
81.90	939.0
83.00	107.0
86.00	278.0
86.90	4913.0
87.90	4623.0
90.80	436.0
91.90	2942.0
92.90	4614.0
94.00	12983.0
95.00	103808.0
96.00	7237.0
96.90	235.0
103.90	585.0
104.80	174.0
105.80	496.0
106.90	120.0
110.80	175.0
113.00	106.0
115.00	104.0
115.90	520.0
116.90	671.0
117.80	426.0
118.90	590.0
127.70	377.0
128.80	229.0
129.80	346.0
130.80	160.0
134.80	218.0
136.80	173.0
140.90	1176.0
141.80	114.0
142.90	1339.0
144.90	248.0
145.80	158.0
147.70	303.0
149.70	113.0
152.80	114.0
154.80	346.0
156.90	262.0
158.60	106.0
160.90	125.0
170.80	128.0
171.90	885.0
173.90	83216.0
175.00	6556.0
175.90	80784.0
177.00	5264.0
177.80	177.0

Instrument :
MSVOA_V
ClientSampleId :
BFB222

m/z	Abundance
36.00	890.0
36.90	4851.0
37.90	3983.0
39.00	1858.0
40.00	243.0
43.90	911.0
44.90	841.0
45.90	186.0
46.90	1077.0
47.90	865.0
48.90	4038.0
50.00	19072.0
51.00	5750.0
52.00	306.0
52.90	106.0
54.90	285.0
55.90	1646.0
57.00	2796.0
57.80	161.0
58.90	115.0
60.00	1012.0
61.00	4826.0
62.00	4827.0
63.00	3801.0
63.90	448.0
65.00	541.0
67.00	291.0
68.00	9708.0
69.00	10262.0
69.90	1052.0
71.90	671.0
73.00	4620.0
74.00	16960.0
75.00	49464.0
76.00	3655.0
76.90	647.0
77.90	466.0
78.90	3422.0
79.90	1007.0
80.90	3662.0
81.80	922.0
82.90	121.0
86.00	232.0
86.90	4450.0
87.90	4143.0
90.80	422.0
92.00	2636.0
92.90	4305.0
94.00	11632.0
95.00	94160.0
96.00	6434.0
97.00	171.0
103.80	553.0
104.80	174.0
105.70	425.0
106.90	122.0
110.80	155.0
115.90	471.0
116.90	628.0
117.80	388.0
118.80	563.0
127.70	400.0
128.80	192.0
129.80	347.0
130.70	117.0
134.80	218.0
136.90	173.0
140.90	1117.0
142.90	1282.0
144.90	183.0
145.80	132.0
147.80	281.0
152.80	118.0
154.80	312.0
156.90	251.0
158.70	105.0
161.00	112.0
170.90	121.0
171.90	828.0
173.90	78440.0
175.00	5918.0
175.90	76152.0
176.90	4753.0
177.80	169.0

Instrument :
MSVOA_V
ClientSampleId :
BFB222