


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV101918\
 Data File : VV008355.D
 Acq On : 19 Oct 2018 09:00
 Operator : SY/MD
 Sample : BFB89
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB89

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR101518WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Sat Oct 20 02:49:28 2018

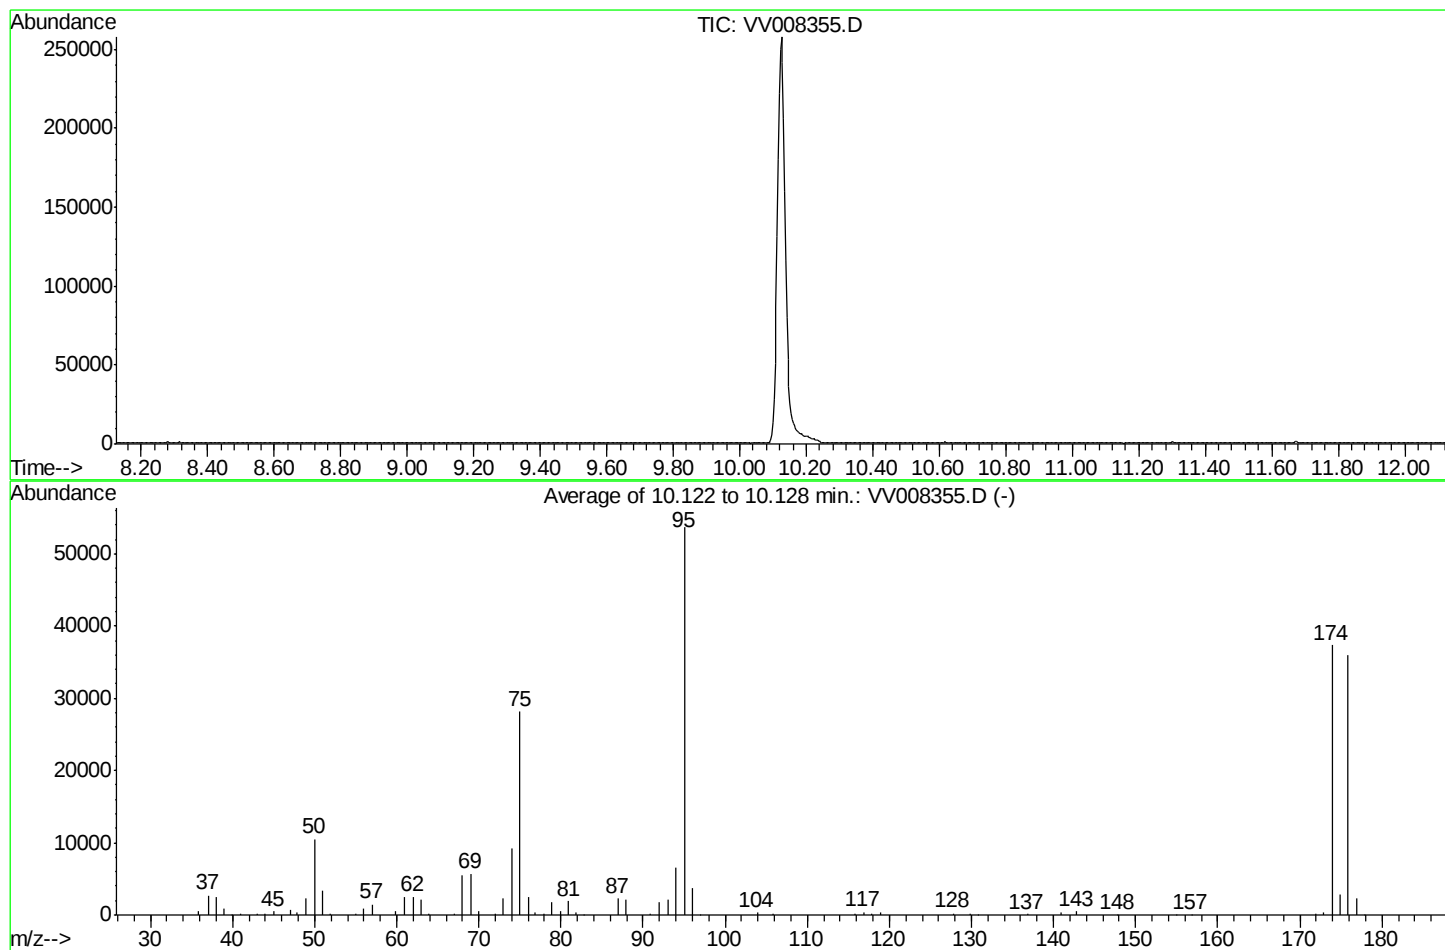

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	10474	PASS
75	95	30	80	52.5	28170	PASS
95	95	100	100	100.0	53666	PASS
96	95	5	9	6.9	3679	PASS
173	174	0.00	2	1.1	424	PASS
174	95	50	120	69.6	37362	PASS
175	174	5	9	7.7	2870	PASS
176	174	95	101	96.2	35946	PASS
177	176	5	9	6.4	2309	PASS

Scan 2796 (10.080 min): VV008355.D
BFB89

m/z	Abundance
39.90	122.0
44.00	431.0

Instrument :
MSVOA_V
ClientSampleId :
BFB89

m/z	Abundance
35.90	513.0
37.00	2752.0
38.00	2415.0
39.00	983.0
39.90	167.0
40.90	116.0
42.90	151.0
43.90	683.0
45.00	508.0
47.00	688.0
47.90	365.0
49.00	2379.0
50.00	10708.0
51.00	3480.0
52.00	203.0
54.90	232.0
56.00	889.0
57.00	1447.0
59.90	473.0
61.00	2381.0
62.00	2459.0
63.00	2138.0
64.00	237.0
67.00	154.0
68.00	5740.0
69.00	5864.0
70.00	491.0
72.00	239.0
73.00	2346.0
74.00	9094.0
75.00	28296.0
76.00	2545.0
76.90	420.0
77.80	233.0
78.90	1780.0
79.90	482.0
80.90	1993.0
81.90	386.0
82.80	107.0
86.90	2249.0
88.00	2082.0
90.90	230.0
91.90	1826.0
93.00	2111.0
94.00	6634.0
95.00	54048.0
96.00	3856.0
96.90	101.0
103.90	327.0
105.80	243.0
115.80	202.0
116.90	383.0
117.90	194.0
118.90	296.0
127.80	177.0
129.80	154.0
136.80	106.0
140.90	402.0
142.90	502.0
156.80	102.0
172.00	173.0
172.90	411.0
173.90	36640.0
174.90	2870.0
175.90	34840.0
176.90	2414.0
177.80	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB89

m/z	Abundance
35.90	518.0
37.00	2711.0
38.00	2500.0
39.00	1016.0
39.90	190.0
41.00	107.0
42.90	174.0
43.90	698.0
45.00	497.0
47.00	731.0
47.90	353.0
48.90	2382.0
50.00	10671.0
51.00	3572.0
51.90	188.0
55.00	201.0
56.00	831.0
57.00	1548.0
59.90	493.0
61.00	2543.0
62.00	2543.0
63.00	2170.0
63.90	234.0
66.90	160.0
68.00	5591.0
69.00	5941.0
70.00	572.0
72.00	276.0
73.00	2376.0
74.00	9483.0
75.00	29120.0
76.00	2534.0
76.90	414.0
77.80	233.0
78.90	1754.0
79.90	533.0
80.90	1939.0
81.90	346.0
86.90	2352.0
88.00	2100.0
90.90	251.0
91.90	1751.0
93.00	2234.0
94.00	6779.0
95.00	55416.0
96.00	3764.0
103.90	317.0
105.80	262.0
115.90	229.0
116.90	376.0
117.90	234.0
118.90	295.0
127.80	199.0
129.80	160.0
136.80	108.0
140.90	421.0
142.80	509.0
147.80	118.0
155.00	110.0
156.80	112.0
172.00	175.0
172.90	423.0
173.90	38664.0
175.00	2990.0
175.90	36960.0
176.90	2398.0
177.90	115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB89

m/z	Abundance
35.00	456.0
37.00	2534.0
38.00	2419.0
39.00	934.0
39.00	191.0
41.00	111.0
43.00	193.0
43.00	675.0
45.00	471.0
47.00	676.0
47.00	300.0
48.00	2138.0
50.00	10044.0
51.00	3331.0
51.00	185.0
55.00	213.0
56.00	738.0
57.00	1471.0
59.00	485.0
61.00	2424.0
62.00	2508.0
63.00	1899.0
63.00	207.0
66.00	164.0
68.00	5015.0
69.00	5381.0
70.00	542.0
72.00	271.0
73.00	2254.0
74.00	8983.0
75.00	27096.0
76.00	2244.0
76.00	384.0
77.00	231.0
78.00	1555.0
79.00	514.0
80.00	1770.0
81.00	283.0
86.00	2206.0
87.00	2036.0
90.00	229.0
91.00	1510.0
93.00	2138.0
94.00	6258.0
95.00	51536.0
96.00	3418.0
104.00	262.0
105.00	288.0
115.00	214.0
116.00	341.0
117.00	230.0
118.00	258.0
127.00	192.0
129.00	146.0
130.00	108.0
136.00	114.0
140.00	469.0
142.00	472.0
147.00	120.0
172.00	143.0
173.00	439.0
173.00	36784.0
175.00	2752.0
175.00	36040.0
176.00	2116.0

Instrument :
MSVOA_V
ClientSampleId :
BFB89