

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101920\
 Data File : VV018970.D
 Acq On : 19 Oct 2020 15:11
 Operator : SY/MD
 Sample : L4426-18 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3Z7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	86	rVB	183347	180675	5.06%	1.368%
2	1.579	145	152	166	rVB	162194	183258	5.14%	1.388%
3	2.123	311	321	351	rVB	318294	494478	13.86%	3.745%
4	2.528	439	447	455	rBV5	1477	2795	0.08%	0.021%
5	2.840	541	544	546	rBV2	394	268	0.01%	0.002%
6	2.920	566	569	572	rBV	346	242	0.01%	0.002%
7	3.119	628	631	633	rBV2	549	287	0.01%	0.002%
8	3.235	665	667	671	rBV2	280	222	0.01%	0.002%
9	3.377	708	711	713	rBV2	465	267	0.01%	0.002%
10	3.479	740	743	745	rBV	346	238	0.01%	0.002%
11	3.563	764	769	771	rBV	456	366	0.01%	0.003%
12	3.589	776	777	781	rBV	238	187	0.01%	0.001%
13	3.836	853	854	856	rVB	179	64	0.00%	0.000%
14	3.852	856	859	861	rBV	264	122	0.00%	0.001%
15	3.865	861	863	865	rBV2	148	91	0.00%	0.001%
16	3.910	867	877	920	rBV	86037	259879	7.28%	1.968%
17	4.312	999	1002	1005	rBV4	362	266	0.01%	0.002%
18	4.376	1005	1022	1051	rVV	197876	495905	13.90%	3.756%
19	4.711	1123	1126	1129	rVB	299	188	0.01%	0.001%
20	4.727	1129	1131	1135	rBV2	310	200	0.01%	0.002%
21	4.762	1135	1142	1144	rBV2	374	331	0.01%	0.003%
22	4.801	1152	1154	1156	rVB	235	78	0.00%	0.001%
23	4.817	1156	1159	1160	rBV	120	70	0.00%	0.001%
24	4.823	1160	1161	1164	rVB2	146	63	0.00%	0.000%
25	4.856	1169	1171	1172	rVV	425	196	0.01%	0.001%
26	4.878	1175	1178	1180	rVB2	269	149	0.00%	0.001%
27	4.894	1180	1183	1187	rBV	202	138	0.00%	0.001%
28	4.917	1187	1190	1194	rBV3	302	234	0.01%	0.002%
29	4.936	1194	1196	1198	rBV3	199	76	0.00%	0.001%
30	5.071	1221	1238	1273	rBV2	475961	1234312	34.59%	9.348%
31	5.302	1308	1310	1311	rBV	444	143	0.00%	0.001%
32	5.434	1350	1351	1352	rBV	257	66	0.00%	0.000%
33	5.460	1356	1359	1362	rBV	290	250	0.01%	0.002%
34	5.511	1372	1375	1377	rBV3	653	379	0.01%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101920\
 Data File : VV018970.D
 Acq On : 19 Oct 2020 15:11
 Operator : SY/MD
 Sample : L4426-18 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3Z7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

35	5.585	1394	1398	1402	rVB2	401	333	0.01%	0.003%
36	5.640	1402	1415	1444	rBV	382299	761368	21.34%	5.766%
37	5.872	1485	1487	1491	rVB	324	166	0.00%	0.001%
38	5.936	1491	1507	1528	rBV4	104170	244734	6.86%	1.853%
39	6.045	1540	1541	1543	rBV	278	96	0.00%	0.001%
40	6.093	1543	1556	1581	rVV	280403	569369	15.96%	4.312%
41	6.286	1613	1616	1617	rBV2	477	255	0.01%	0.002%
42	6.357	1636	1638	1641	rBV2	294	152	0.00%	0.001%
43	6.380	1642	1645	1647	rVB2	271	144	0.00%	0.001%
44	6.409	1652	1654	1660	rBV2	323	311	0.01%	0.002%
45	6.434	1660	1662	1664	rBV	153	73	0.00%	0.001%
46	6.508	1681	1685	1690	rVB3	347	259	0.01%	0.002%
47	6.550	1695	1698	1699	rBV	129	74	0.00%	0.001%
48	6.560	1699	1701	1704	rVB2	348	210	0.01%	0.002%
49	6.659	1727	1732	1734	rBV2	458	424	0.01%	0.003%
50	6.688	1739	1741	1743	rBV2	333	159	0.00%	0.001%
51	6.737	1752	1756	1758	rBV2	383	276	0.01%	0.002%
52	6.769	1762	1766	1771	rBV	374	387	0.01%	0.003%
53	6.807	1775	1778	1781	rBV2	374	194	0.01%	0.001%
54	6.872	1795	1798	1801	rBV	298	247	0.01%	0.002%
55	6.891	1801	1804	1805	rBV	346	188	0.01%	0.001%
56	6.968	1826	1828	1829	rBV	296	131	0.00%	0.001%
57	7.007	1830	1840	1862	rVV	148439	268716	7.53%	2.035%
58	7.338	1931	1943	1969	rBV	547933	949006	26.60%	7.187%
59	7.643	2028	2038	2059	rBV	106784	189301	5.31%	1.434%
60	7.826	2093	2095	2099	rBV2	324	203	0.01%	0.002%
61	7.846	2099	2101	2104	rBV3	440	257	0.01%	0.002%
62	7.881	2109	2112	2116	rBV2	375	274	0.01%	0.002%
63	7.929	2125	2127	2129	rVB	293	108	0.00%	0.001%
64	7.997	2134	2148	2172	rBV	2157182	3568345	100.00%	27.024%
65	8.109	2173	2183	2217	rVB2	271708	560965	15.72%	4.248%
66	8.399	2271	2273	2274	rBV	502	214	0.01%	0.002%
67	8.431	2281	2283	2284	rBV	473	183	0.01%	0.001%
68	8.505	2303	2306	2309	rBV3	615	398	0.01%	0.003%
69	8.871	2408	2420	2447	rBV	602454	966141	27.08%	7.317%
70	9.077	2479	2484	2488	rBV4	650	687	0.02%	0.005%
71	9.097	2488	2490	2491	rBV	358	130	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101920\
 Data File : VV018970.D
 Acq On : 19 Oct 2020 15:11
 Operator : SY/MD
 Sample : L4426-18 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3Z7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

72	9.579	2638	2640	2642	rBV	245	153	0.00%	0.001%
73	9.598	2645	2646	2647	rBV	155	49	0.00%	0.000%
74	9.695	2673	2676	2678	rBV2	475	231	0.01%	0.002%
75	9.707	2678	2680	2683	rBV	376	260	0.01%	0.002%
76	9.772	2697	2700	2704	rBV	278	233	0.01%	0.002%
77	9.826	2714	2717	2719	rBV	273	178	0.00%	0.001%
78	9.836	2719	2720	2722	rVV	208	82	0.00%	0.001%
79	9.887	2730	2736	2738	rBV	403	429	0.01%	0.003%
80	9.936	2748	2751	2754	rBV3	377	319	0.01%	0.002%
81	9.952	2754	2756	2760	rVV2	421	291	0.01%	0.002%
82	10.235	2832	2844	2864	rBV	288712	454071	12.72%	3.439%
83	10.373	2884	2887	2890	rBV	304	187	0.01%	0.001%
84	10.431	2901	2905	2909	rBV3	365	382	0.01%	0.003%
85	10.511	2927	2930	2932	rBV2	366	197	0.01%	0.001%
86	10.569	2946	2948	2951	rBV	243	187	0.01%	0.001%
87	10.675	2978	2981	2983	rBV3	381	258	0.01%	0.002%
88	10.958	3067	3069	3071	rVB	311	104	0.00%	0.001%
89	11.170	3133	3135	3136	rBV	264	104	0.00%	0.001%
90	11.270	3155	3166	3187	rBV	585685	891995	25.00%	6.755%
91	11.646	3270	3283	3306	rBV	588259	912303	25.57%	6.909%
92	12.106	3424	3426	3429	rBV2	316	185	0.01%	0.001%
93	12.704	3610	3612	3613	rBV2	346	148	0.00%	0.001%
94	13.485	3852	3855	3857	rBV	423	242	0.01%	0.002%
95	13.964	4000	4004	4005	rBV2	388	344	0.01%	0.003%
96	14.016	4014	4020	4022	rBV4	618	622	0.02%	0.005%


Sum of corrected areas: 13204515

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV101920\
Data File : VV018970.D
Acq On : 19 Oct 2020 15:11
Operator : SY/MD
Sample : L4426-18 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3Z7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

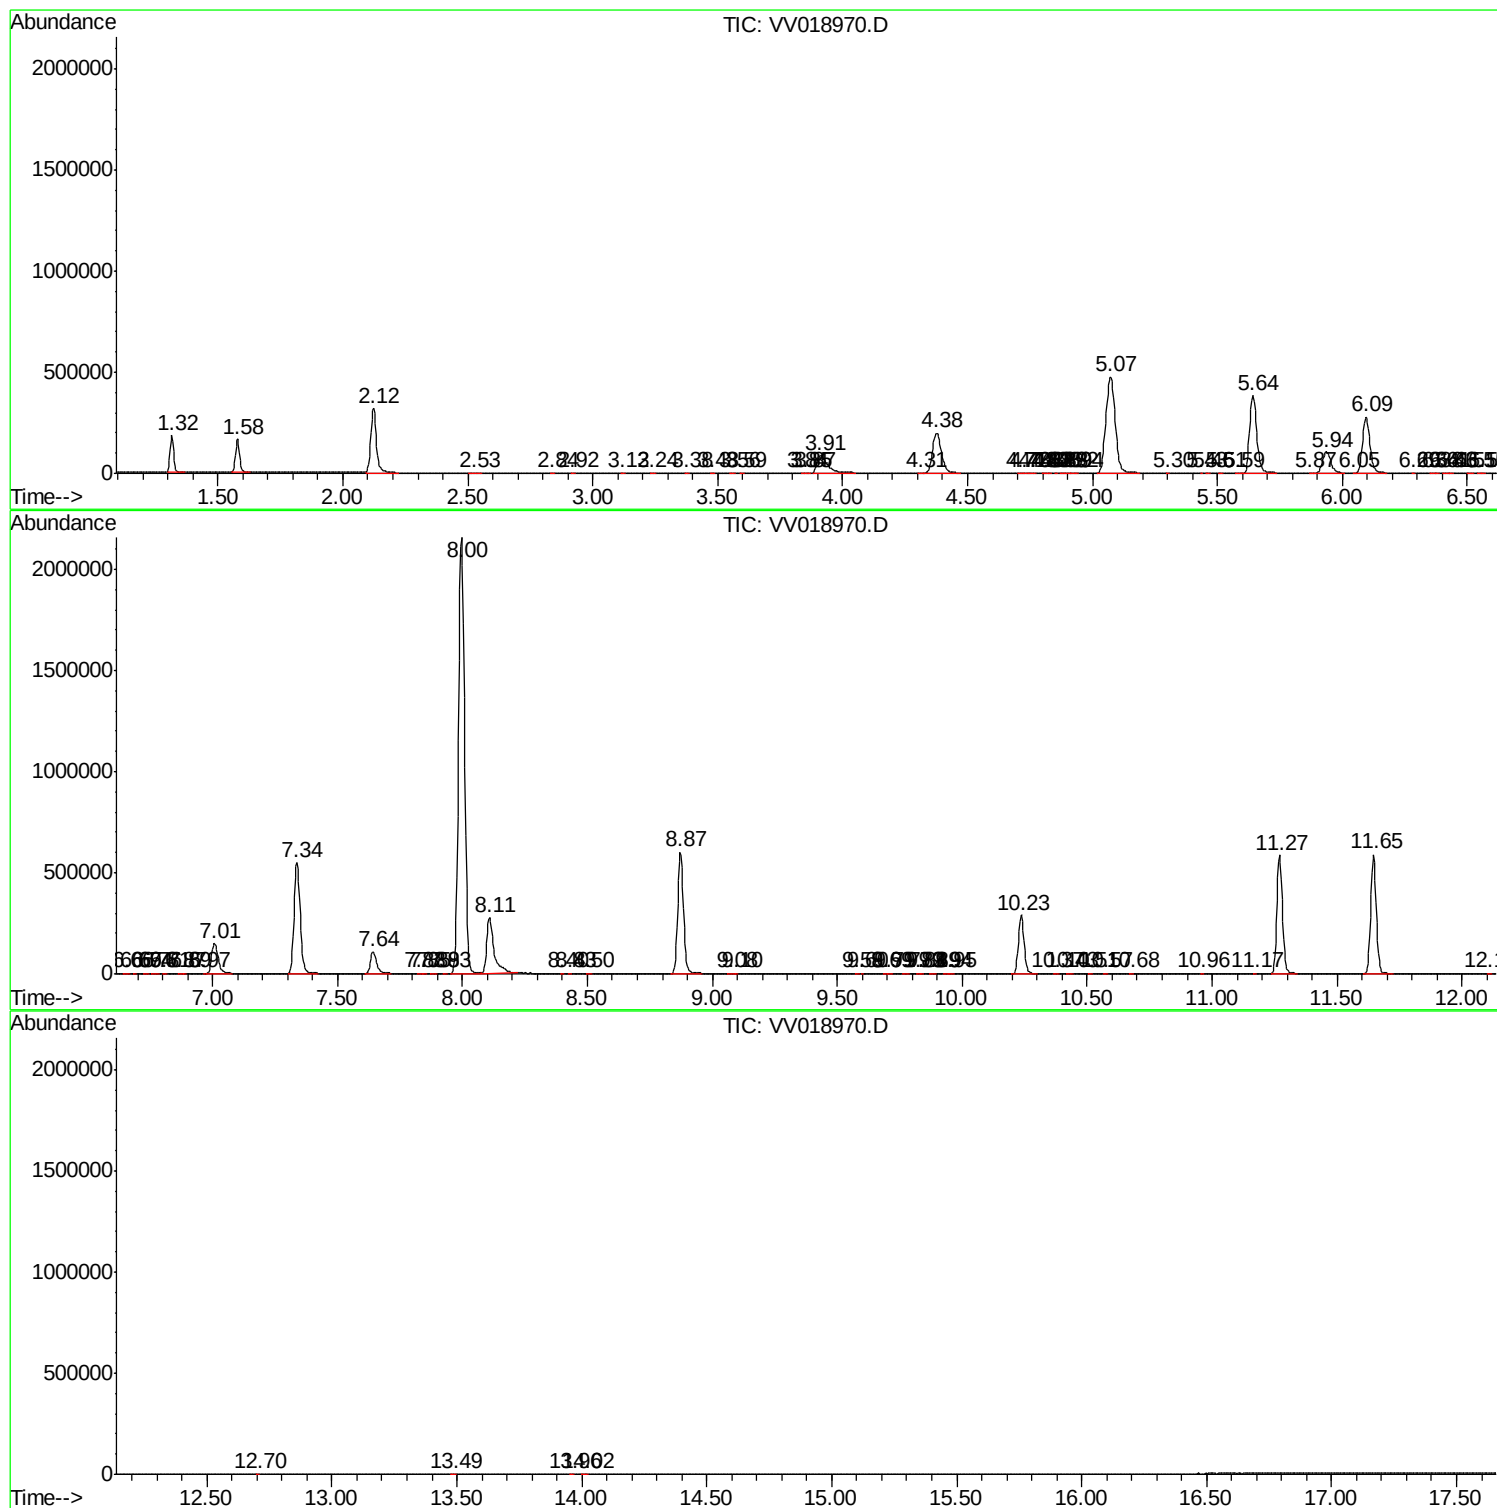

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV101920\
Data File : VV018970.D
Acq On : 19 Oct 2020 15:11
Operator : SY/MD
Sample : L4426-18 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3Z7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV101920\
Data File : VV018970.D
Acq On : 19 Oct 2020 15:11
Operator : SY/MD
Sample : L4426-18 100X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BG3Z7

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc