

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101920\
 Data File : VV018973.D
 Acq On : 19 Oct 2020 16:22
 Operator : SY/MD
 Sample : L4426-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3Z5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	86	rVB	177049	174292	13.49%	1.748%
2	1.579	145	152	163	rBV	159158	180069	13.94%	1.806%
3	2.122	312	321	347	rVB	303683	460636	35.65%	4.621%
4	2.682	490	495	497	rBV3	740	684	0.05%	0.007%
5	2.753	513	517	520	rBV3	637	557	0.04%	0.006%
6	2.958	579	581	582	rBV	278	108	0.01%	0.001%
7	3.055	609	611	613	rBV	452	240	0.02%	0.002%
8	3.132	631	635	638	rBV2	286	322	0.02%	0.003%
9	3.447	731	733	736	rBV	411	231	0.02%	0.002%
10	3.508	750	752	754	rVB	293	127	0.01%	0.001%
11	3.524	754	757	758	rBV	487	254	0.02%	0.003%
12	3.553	763	766	768	rBV	215	140	0.01%	0.001%
13	3.647	794	795	799	rVB	246	98	0.01%	0.001%
14	3.743	821	825	827	rBV	280	185	0.01%	0.002%
15	3.917	868	879	918	rBV	86967	278129	21.53%	2.790%
16	4.376	1007	1022	1051	rVB	208503	513112	39.72%	5.147%
17	4.769	1142	1144	1145	rBV	233	86	0.01%	0.001%
18	4.827	1159	1162	1163	rBV	179	111	0.01%	0.001%
19	4.881	1177	1179	1182	rBV2	415	216	0.02%	0.002%
20	5.071	1221	1238	1269	rBV2	496635	1291956	100.00%	12.961%
21	5.454	1354	1357	1362	rVB2	934	611	0.05%	0.006%
22	5.495	1369	1370	1374	rVB2	488	208	0.02%	0.002%
23	5.582	1393	1397	1403	rBV3	412	461	0.04%	0.005%
24	5.640	1403	1415	1441	rBV	405245	810100	62.70%	8.127%
25	5.875	1486	1488	1490	rVB3	605	202	0.02%	0.002%
26	5.929	1493	1505	1527	rBV2	32336	70271	5.44%	0.705%
27	6.093	1543	1556	1580	rBV	291823	590455	45.70%	5.923%
28	6.232	1597	1599	1600	rBV2	584	245	0.02%	0.002%
29	6.363	1638	1640	1641	rBV	233	101	0.01%	0.001%
30	6.386	1645	1647	1650	rBV2	507	238	0.02%	0.002%
31	6.527	1685	1691	1692	rBV2	422	272	0.02%	0.003%
32	6.540	1693	1695	1698	rVB2	493	242	0.02%	0.002%
33	6.563	1698	1702	1705	rBV2	306	270	0.02%	0.003%
34	6.592	1709	1711	1713	rVB2	331	164	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101920\
 Data File : VV018973.D
 Acq On : 19 Oct 2020 16:22
 Operator : SY/MD
 Sample : L4426-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3Z5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

35	6.717	1749	1750	1755	rVB2	557	331	0.03%	0.003%
36	6.769	1765	1766	1767	rBV2	270	93	0.01%	0.001%
37	7.007	1829	1840	1867	rBV	140018	257545	19.93%	2.584%
38	7.203	1897	1901	1903	rBV2	518	424	0.03%	0.004%
39	7.296	1927	1930	1931	rBV	317	167	0.01%	0.002%
40	7.338	1931	1943	1964	rBV	533627	917767	71.04%	9.207%
41	7.643	2026	2038	2064	rBV	96500	174162	13.48%	1.747%
42	7.833	2095	2097	2098	rBV	375	147	0.01%	0.001%
43	7.871	2108	2109	2112	rBV	121	58	0.00%	0.001%
44	7.997	2137	2148	2165	rVB	272877	451854	34.97%	4.533%
45	8.109	2173	2183	2221	rBV3	253307	546118	42.27%	5.479%
46	8.527	2309	2313	2316	rBV3	321	255	0.02%	0.003%
47	8.621	2340	2342	2344	rBV2	235	141	0.01%	0.001%
48	8.646	2347	2350	2351	rBV2	223	127	0.01%	0.001%
49	8.727	2373	2375	2377	rVB2	141	60	0.00%	0.001%
50	8.749	2377	2382	2385	rBV	535	436	0.03%	0.004%
51	8.823	2399	2405	2408	rBV2	289	325	0.03%	0.003%
52	8.871	2408	2420	2447	rBV	594882	969393	75.03%	9.725%
53	9.113	2493	2495	2496	rBV	127	47	0.00%	0.000%
54	9.129	2498	2500	2507	rVB	409	307	0.02%	0.003%
55	9.158	2507	2509	2511	rBV2	298	145	0.01%	0.001%
56	9.183	2516	2517	2518	rBV2	197	49	0.00%	0.000%
57	9.264	2537	2542	2544	rBV2	383	330	0.03%	0.003%
58	9.376	2574	2577	2579	rBV2	411	208	0.02%	0.002%
59	9.450	2595	2600	2605	rBV2	417	402	0.03%	0.004%
60	9.511	2615	2619	2627	rBV2	483	624	0.05%	0.006%
61	9.608	2646	2649	2653	rVB2	228	142	0.01%	0.001%
62	9.643	2658	2660	2661	rVB2	121	29	0.00%	0.000%
63	9.662	2662	2666	2670	rVB3	517	420	0.03%	0.004%
64	9.691	2670	2675	2678	rBV	348	326	0.03%	0.003%
65	9.730	2685	2687	2688	rBV	144	41	0.00%	0.000%
66	9.781	2700	2703	2705	rBV	252	145	0.01%	0.001%
67	9.910	2740	2743	2746	rBV	252	153	0.01%	0.002%
68	9.929	2746	2749	2750	rBV2	143	76	0.01%	0.001%
69	10.000	2761	2771	2773	rBV2	443	713	0.06%	0.007%
70	10.032	2777	2781	2784	rVB2	441	317	0.02%	0.003%
71	10.051	2784	2787	2788	rBV	208	99	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101920\
 Data File : VV018973.D
 Acq On : 19 Oct 2020 16:22
 Operator : SY/MD
 Sample : L4426-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3Z5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

72	10.077	2792	2795	2796	rBV2	273	135	0.01%	0.001%
73	10.116	2804	2807	2810	rBV	228	189	0.01%	0.002%
74	10.190	2824	2830	2831	rBV	257	234	0.02%	0.002%
75	10.238	2833	2845	2867	rVV	304880	480047	37.16%	4.816%
76	10.402	2888	2896	2909	rVB3	4041	6437	0.50%	0.065%
77	10.588	2952	2954	2957	rBV2	387	284	0.02%	0.003%
78	10.637	2966	2969	2970	rBV2	350	179	0.01%	0.002%
79	10.717	2990	2994	2997	rBV2	402	327	0.03%	0.003%
80	10.794	3015	3018	3020	rBV2	258	160	0.01%	0.002%
81	10.842	3031	3033	3036	rBV2	294	154	0.01%	0.002%
82	10.961	3067	3070	3072	rBV2	203	99	0.01%	0.001%
83	11.045	3091	3096	3097	rBV2	259	225	0.02%	0.002%
84	11.141	3124	3126	3132	rBV	236	167	0.01%	0.002%
85	11.270	3154	3166	3190	rBV	577864	894916	69.27%	8.978%
86	11.489	3231	3234	3239	rVB2	667	430	0.03%	0.004%
87	11.518	3239	3243	3245	rBV2	458	346	0.03%	0.003%
88	11.569	3251	3259	3262	rBV5	988	1231	0.10%	0.012%
89	11.646	3271	3283	3306	rBV	560666	881418	68.22%	8.842%
90	12.074	3413	3416	3420	rBV	467	290	0.02%	0.003%
91	12.492	3542	3546	3548	rBV	368	273	0.02%	0.003%
92	13.315	3801	3802	3803	rBV	245	93	0.01%	0.001%
93	13.405	3827	3830	3833	rBV2	327	236	0.02%	0.002%
94	13.733	3928	3932	3936	rBV3	666	631	0.05%	0.006%
95	13.984	4006	4010	4013	rBV	493	442	0.03%	0.004%


Sum of corrected areas: 9968312

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV101920\
Data File : VV018973.D
Acq On : 19 Oct 2020 16:22
Operator : SY/MD
Sample : L4426-04
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
BG3Z5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

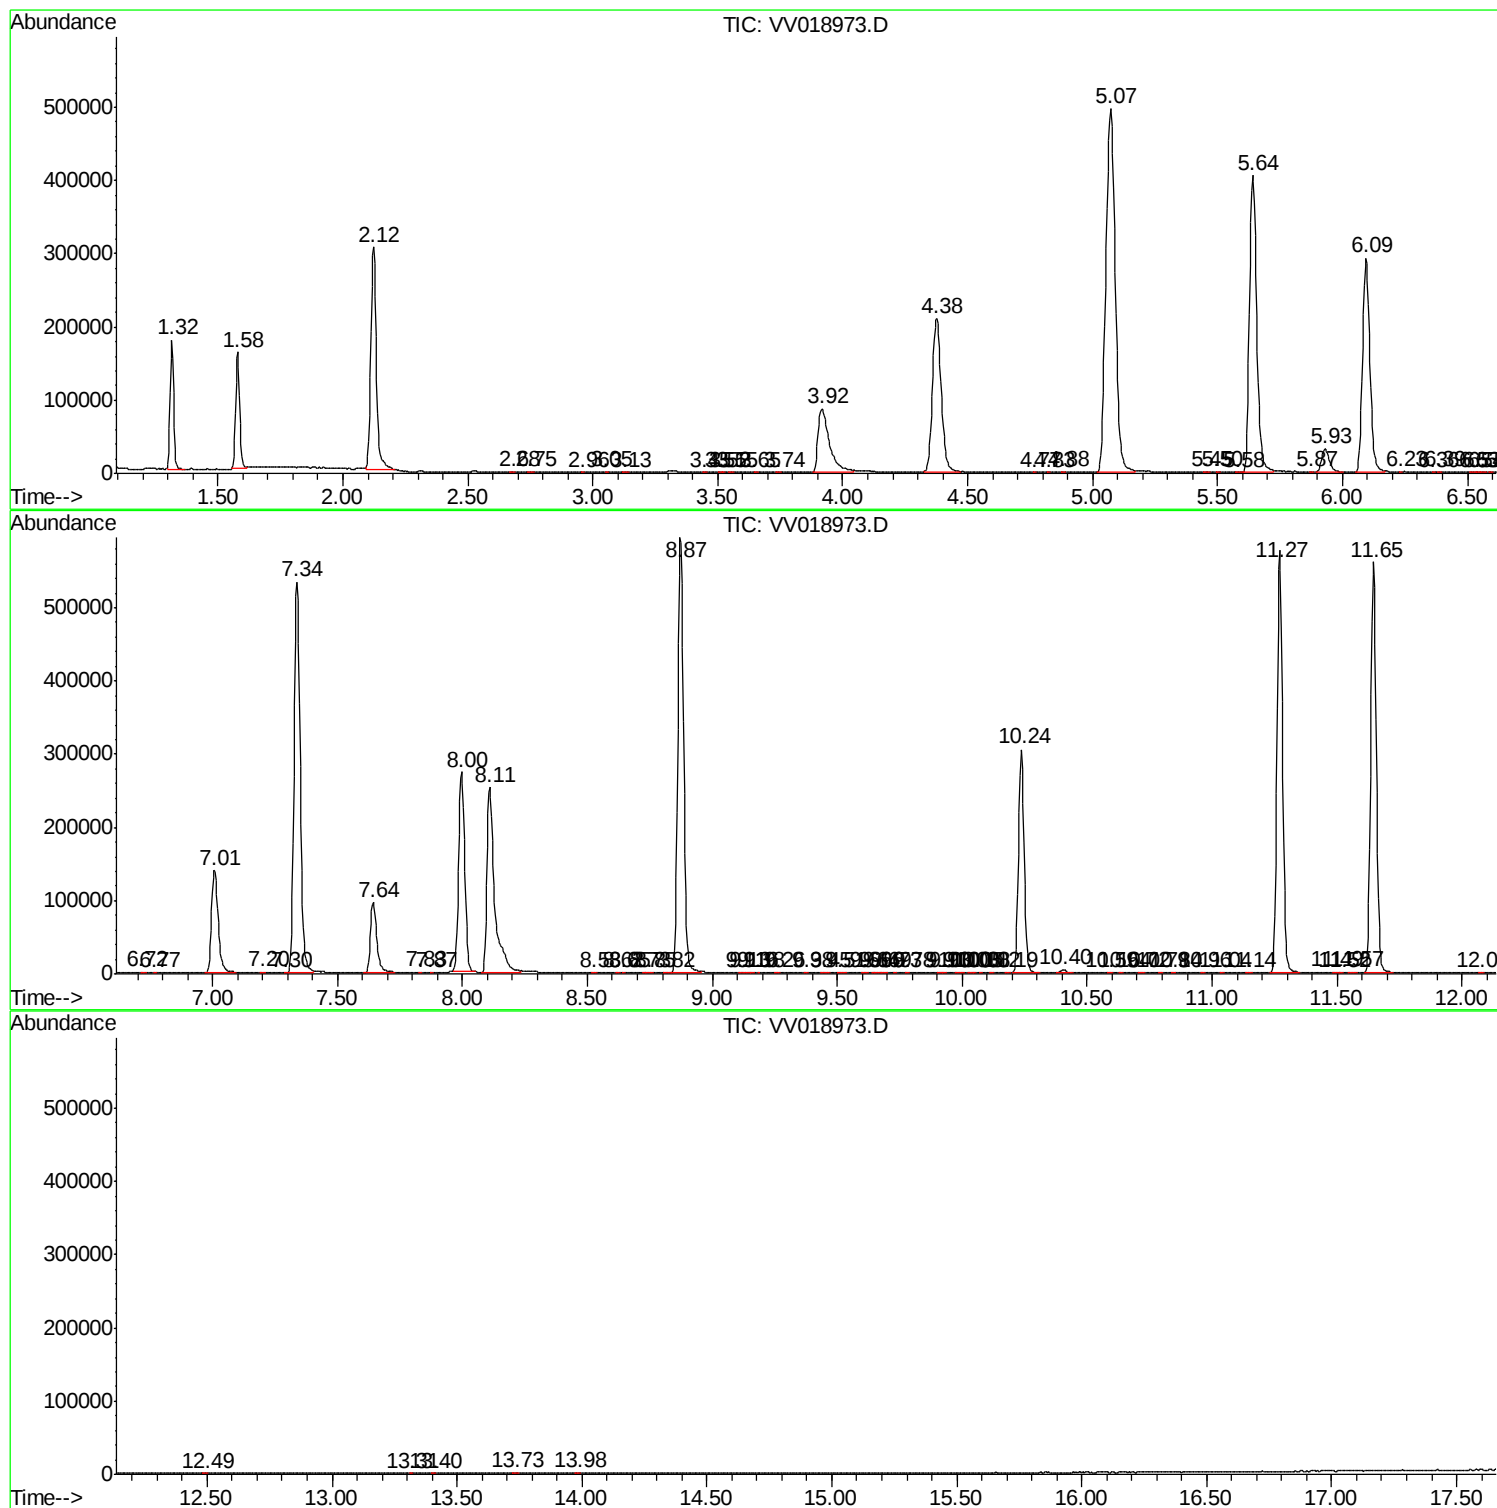

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV101920\
Data File : VV018973.D
Acq On : 19 Oct 2020 16:22
Operator : SY/MD
Sample : L4426-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3Z5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV101920\
Data File : VV018973.D
Acq On : 19 Oct 2020 16:22
Operator : SY/MD
Sample : L4426-04
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BG3Z5

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc