

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101920\
 Data File : VV018980.D
 Acq On : 19 Oct 2020 19:07
 Operator : SY/MD
 Sample : L4426-20
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG413

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.225	38	42	47	rVB2	10279	8255	0.68%	0.089%
2	1.315	64	70	83	rVB	167658	171503	14.17%	1.839%
3	1.579	145	152	165	rVB	153592	172169	14.23%	1.846%
4	2.122	312	321	341	rBV	294728	442948	36.61%	4.749%
5	2.637	478	481	486	rVB	419	330	0.03%	0.004%
6	2.663	486	489	492	rBV3	437	310	0.03%	0.003%
7	2.675	492	493	494	rBV	451	111	0.01%	0.001%
8	2.714	504	505	508	rVB3	445	191	0.02%	0.002%
9	2.929	570	572	579	rVB4	410	282	0.02%	0.003%
10	2.974	580	586	589	rBV2	683	623	0.05%	0.007%
11	3.100	623	625	628	rVB2	349	132	0.01%	0.001%
12	3.116	628	630	632	rBV	336	199	0.02%	0.002%
13	3.161	641	644	647	rBV2	230	125	0.01%	0.001%
14	3.190	652	653	659	rVB	326	192	0.02%	0.002%
15	3.238	665	668	670	rBV	192	138	0.01%	0.001%
16	3.267	674	677	680	rVB	230	138	0.01%	0.001%
17	3.299	683	687	689	rBV	244	160	0.01%	0.002%
18	3.312	689	691	693	rBV	157	82	0.01%	0.001%
19	3.428	723	727	732	rBV2	306	400	0.03%	0.004%
20	3.515	752	754	756	rBV	148	92	0.01%	0.001%
21	3.582	773	775	777	rBV	276	188	0.02%	0.002%
22	3.662	799	800	803	rBV	148	73	0.01%	0.001%
23	3.720	816	818	821	rBV2	183	132	0.01%	0.001%
24	3.736	821	823	825	rVV	238	81	0.01%	0.001%
25	3.752	825	828	831	rVV2	325	208	0.02%	0.002%
26	3.810	842	846	848	rBV	271	208	0.02%	0.002%
27	3.916	868	879	918	rBV	80156	249072	20.59%	2.670%
28	4.376	1005	1022	1053	rBV	193911	484232	40.02%	5.192%
29	4.617	1094	1097	1099	rBV2	496	277	0.02%	0.003%
30	4.756	1138	1140	1141	rBV2	389	113	0.01%	0.001%
31	4.836	1163	1165	1168	rBV2	194	85	0.01%	0.001%
32	4.865	1172	1174	1175	rVV	228	63	0.01%	0.001%
33	4.916	1186	1190	1193	rBV	273	216	0.02%	0.002%
34	4.933	1193	1195	1197	rVV	229	75	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101920\
 Data File : VV018980.D
 Acq On : 19 Oct 2020 19:07
 Operator : SY/MD
 Sample : L4426-20
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG413

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

35	4.955	1199	1202	1204	rBV2	217	124	0.01%	0.001%
36	4.997	1211	1215	1216	rBV	280	179	0.01%	0.002%
37	5.071	1221	1238	1272	rBV2	465486	1209943	100.00%	12.973%
38	5.434	1349	1351	1353	rBV3	331	143	0.01%	0.002%
39	5.450	1353	1356	1358	rBV3	386	212	0.02%	0.002%
40	5.482	1364	1366	1368	rBV	279	145	0.01%	0.002%
41	5.537	1381	1383	1386	rVB	330	123	0.01%	0.001%
42	5.640	1403	1415	1446	rBV	364549	739567	61.12%	7.929%
43	5.878	1487	1489	1493	rBV2	332	217	0.02%	0.002%
44	5.926	1493	1504	1527	rVV2	55364	116223	9.61%	1.246%
45	6.093	1542	1556	1582	rBV2	272025	553755	45.77%	5.937%
46	6.360	1633	1639	1640	rBV2	459	389	0.03%	0.004%
47	6.386	1644	1647	1650	rVB2	530	338	0.03%	0.004%
48	6.408	1651	1654	1659	rVB3	367	306	0.03%	0.003%
49	6.469	1670	1673	1680	rVB3	416	419	0.03%	0.004%
50	6.508	1681	1685	1688	rBV2	437	345	0.03%	0.004%
51	6.540	1692	1695	1697	rBV	392	271	0.02%	0.003%
52	6.588	1704	1710	1714	rBV3	711	1024	0.08%	0.011%
53	6.765	1763	1765	1768	rBV	296	169	0.01%	0.002%
54	6.820	1780	1782	1786	rBV	278	131	0.01%	0.001%
55	6.855	1790	1793	1795	rBV	228	187	0.02%	0.002%
56	6.875	1797	1799	1801	rVV	381	141	0.01%	0.002%
57	6.897	1803	1806	1812	rVB2	395	360	0.03%	0.004%
58	6.961	1823	1826	1827	rBV2	101	56	0.00%	0.001%
59	7.006	1828	1840	1878	rBV	141945	265463	21.94%	2.846%
60	7.338	1931	1943	1965	rBV	534256	926883	76.61%	9.938%
61	7.566	2012	2014	2016	rBV3	456	258	0.02%	0.003%
62	7.643	2027	2038	2058	rBV	103153	182460	15.08%	1.956%
63	7.958	2133	2136	2139	rBV3	629	464	0.04%	0.005%
64	8.003	2144	2150	2159	rBV4	2443	3587	0.30%	0.038%
65	8.061	2165	2168	2170	rBV2	344	229	0.02%	0.002%
66	8.109	2173	2183	2218	rBV3	248248	541210	44.73%	5.803%
67	8.434	2281	2284	2289	rBV	535	450	0.04%	0.005%
68	8.505	2304	2306	2313	rBV2	356	346	0.03%	0.004%
69	8.701	2362	2367	2370	rBV3	253	244	0.02%	0.003%
70	8.723	2370	2374	2376	rBV	302	211	0.02%	0.002%
71	8.871	2409	2420	2446	rBV	575353	936880	77.43%	10.045%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101920\
 Data File : VV018980.D
 Acq On : 19 Oct 2020 19:07
 Operator : SY/MD
 Sample : L4426-20
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG413

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

72	9.122	2494	2498	2501	rBV4	660	564	0.05%	0.006%
73	9.170	2509	2513	2515	rBV2	402	273	0.02%	0.003%
74	9.296	2549	2552	2553	rBV	168	87	0.01%	0.001%
75	9.524	2621	2623	2625	rBV	186	120	0.01%	0.001%
76	9.543	2627	2629	2630	rBV	336	153	0.01%	0.002%
77	9.685	2671	2673	2674	rBV	133	61	0.01%	0.001%
78	9.698	2674	2677	2680	rVB	415	226	0.02%	0.002%
79	9.720	2681	2684	2688	rBV2	352	266	0.02%	0.003%
80	9.772	2697	2700	2705	rVB3	449	387	0.03%	0.004%
81	9.800	2705	2709	2710	rBV	268	189	0.02%	0.002%
82	9.842	2715	2722	2725	rVV3	387	520	0.04%	0.006%
83	10.026	2777	2779	2782	rBV2	334	187	0.02%	0.002%
84	10.051	2785	2787	2790	rBV	164	76	0.01%	0.001%
85	10.083	2795	2797	2799	rBV	227	139	0.01%	0.001%
86	10.096	2799	2801	2806	rBV2	380	294	0.02%	0.003%
87	10.157	2818	2820	2824	rBV	359	269	0.02%	0.003%
88	10.180	2824	2827	2829	rBV	306	128	0.01%	0.001%
89	10.238	2833	2845	2863	rBV	260870	412714	34.11%	4.425%
90	10.399	2891	2895	2904	rVB3	1298	1786	0.15%	0.019%
91	10.653	2971	2974	2979	rVB	318	292	0.02%	0.003%
92	10.964	3063	3071	3076	rBV4	1506	2456	0.20%	0.026%
93	11.270	3154	3166	3191	rBV	605379	940420	77.72%	10.083%
94	11.646	3270	3283	3304	rBV	612258	947265	78.29%	10.156%
95	13.296	3795	3796	3799	rBV	358	242	0.02%	0.003%
96	13.656	3906	3908	3909	rBV	373	166	0.01%	0.002%
97	13.878	3974	3977	3983	rBV3	615	765	0.06%	0.008%


Sum of corrected areas: 9326900

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV101920\
Data File : VV018980.D
Acq On : 19 Oct 2020 19:07
Operator : SY/MD
Sample : L4426-20
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
BG413

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

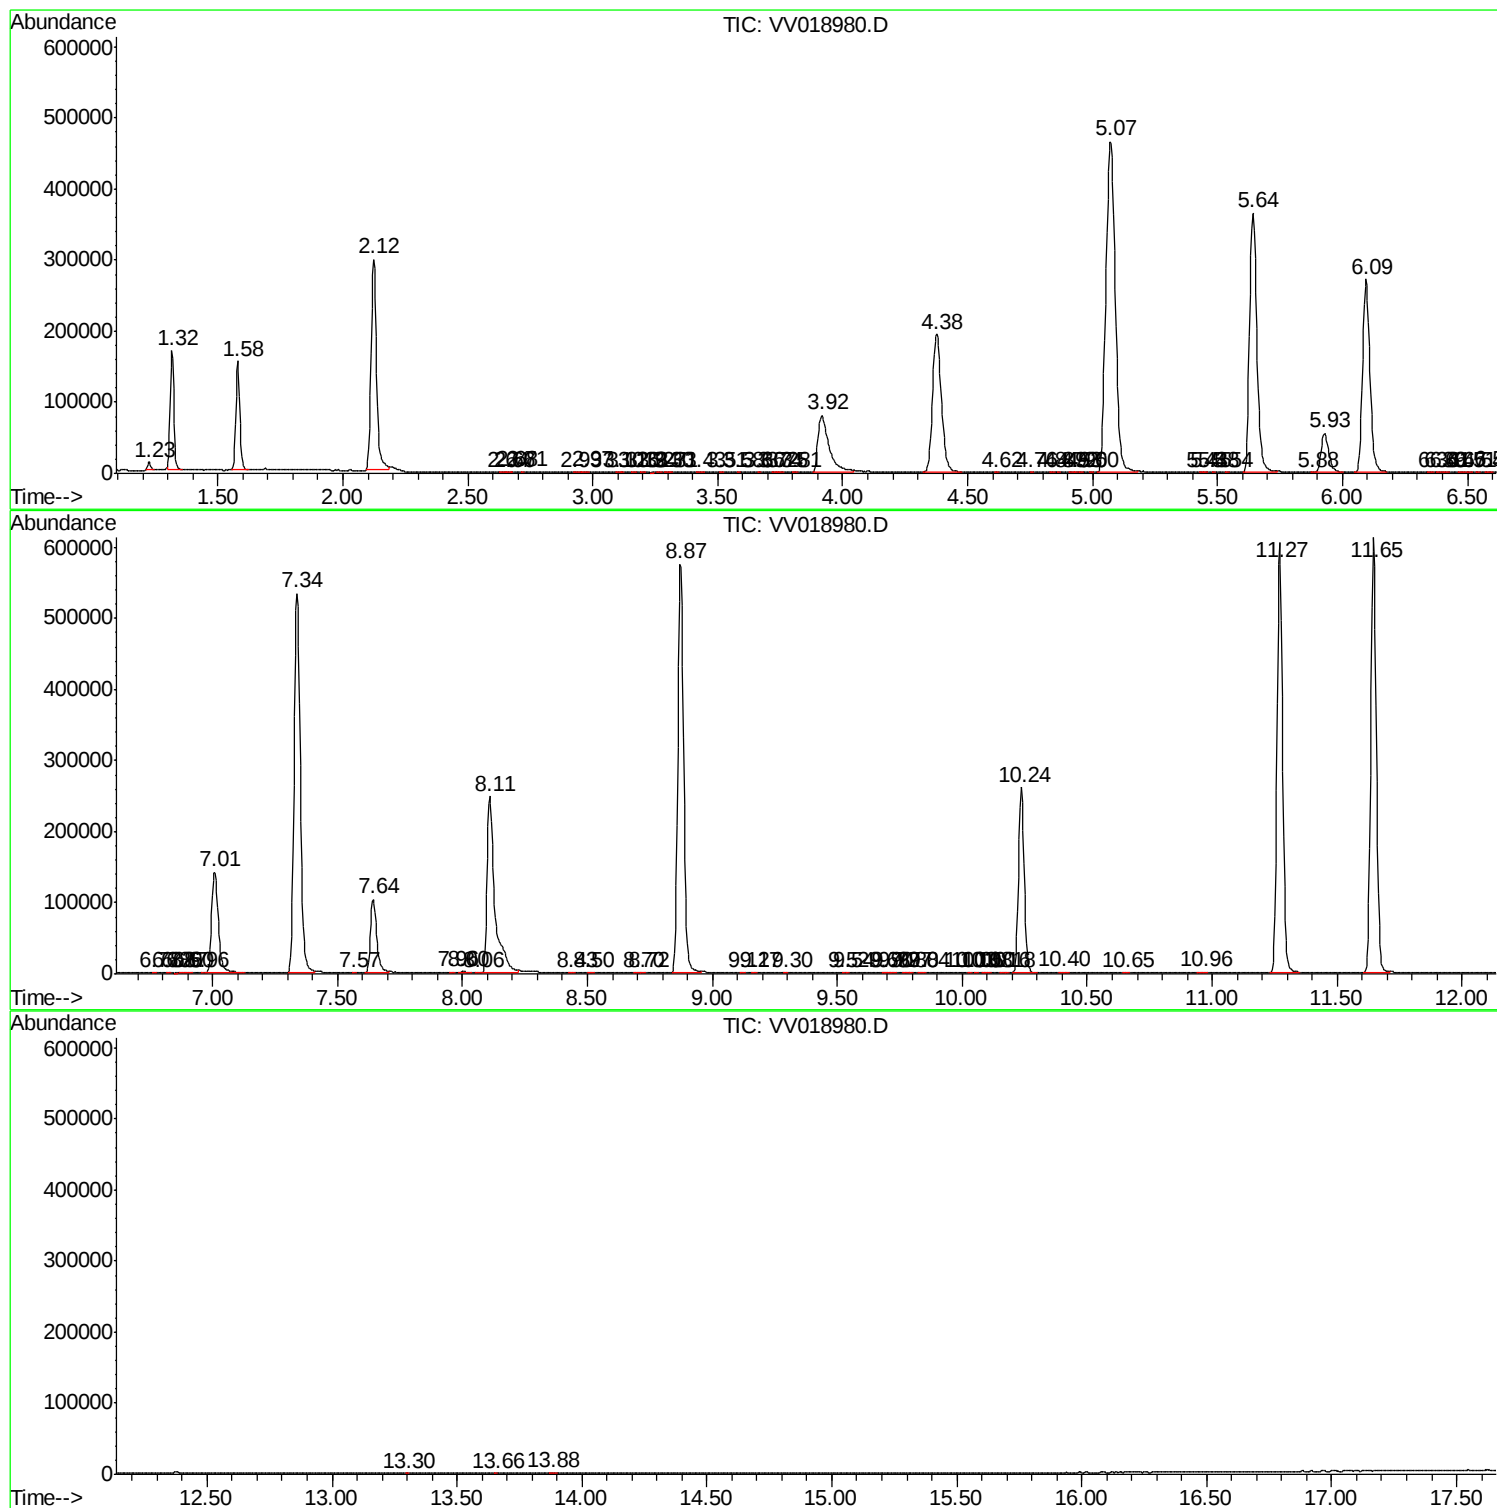

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV101920\
Data File : VV018980.D
Acq On : 19 Oct 2020 19:07
Operator : SY/MD
Sample : L4426-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG413

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV101920\
Data File : VV018980.D
Acq On : 19 Oct 2020 19:07
Operator : SY/MD
Sample : L4426-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG413

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc