

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101920\
 Data File : VV018988.D
 Acq On : 20 Oct 2020 00:45
 Operator : SY/MD
 Sample : L4430-01 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	80	rVB	165344	166577	13.59%	1.829%
2	1.576	144	151	162	rBV	145189	159909	13.05%	1.755%
3	2.119	311	320	347	rVB	282733	436550	35.62%	4.792%
4	2.920	565	569	570	rBV	718	456	0.04%	0.005%
5	3.187	650	652	655	rBV2	497	308	0.03%	0.003%
6	3.476	740	742	743	rBV	350	126	0.01%	0.001%
7	3.711	813	815	821	rVB2	367	341	0.03%	0.004%
8	3.753	826	828	829	rBV2	417	124	0.01%	0.001%
9	3.804	839	844	846	rBV2	434	414	0.03%	0.005%
10	3.910	865	877	910	rBV2	102525	361510	29.50%	3.969%
11	4.373	1004	1021	1049	rBV	199342	502842	41.03%	5.520%
12	4.756	1136	1140	1143	rBV3	598	513	0.04%	0.006%
13	4.807	1153	1156	1157	rBV	454	284	0.02%	0.003%
14	4.949	1199	1200	1201	rBV	211	68	0.01%	0.001%
15	4.981	1207	1210	1213	rBV2	465	342	0.03%	0.004%
16	5.071	1220	1238	1272	rBV2	476455	1225582	100.00%	13.454%
17	5.466	1358	1361	1362	rBV	385	189	0.02%	0.002%
18	5.524	1376	1379	1381	rBV2	352	179	0.01%	0.002%
19	5.576	1389	1395	1398	rBV	599	487	0.04%	0.005%
20	5.640	1400	1415	1444	rBV	361398	721545	58.87%	7.921%
21	5.926	1492	1504	1526	rBV	45627	97137	7.93%	1.066%
22	6.042	1538	1540	1542	rBV2	391	213	0.02%	0.002%
23	6.093	1542	1556	1577	rBV	259854	528585	43.13%	5.803%
24	6.351	1633	1636	1639	rVB	346	184	0.02%	0.002%
25	6.373	1639	1643	1645	rBV3	301	205	0.02%	0.002%
26	6.437	1661	1663	1666	rVB2	250	94	0.01%	0.001%
27	6.460	1668	1670	1672	rBV	154	56	0.00%	0.001%
28	6.482	1673	1677	1678	rVV2	135	87	0.01%	0.001%
29	6.498	1681	1682	1686	rVB2	453	229	0.02%	0.003%
30	6.518	1686	1688	1691	rBV	278	138	0.01%	0.002%
31	6.537	1691	1694	1696	rBV2	149	105	0.01%	0.001%
32	6.550	1696	1698	1703	rVB	279	178	0.01%	0.002%
33	6.588	1707	1710	1711	rBV	265	143	0.01%	0.002%
34	6.659	1730	1732	1734	rBV	201	131	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101920\
 Data File : VV018988.D
 Acq On : 20 Oct 2020 00:45
 Operator : SY/MD
 Sample : L4430-01 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

35	6.724	1749	1752	1756	rBV2	421	413	0.03%	0.005%
36	6.785	1765	1771	1773	rBV2	347	273	0.02%	0.003%
37	6.820	1780	1782	1786	rBV2	163	77	0.01%	0.001%
38	6.878	1797	1800	1805	rVB3	311	225	0.02%	0.002%
39	6.904	1805	1808	1810	rBV	164	97	0.01%	0.001%
40	6.952	1818	1823	1825	rBV2	375	302	0.02%	0.003%
41	7.006	1829	1840	1879	rVV	134585	248791	20.30%	2.731%
42	7.289	1925	1928	1931	rBV2	486	307	0.03%	0.003%
43	7.338	1931	1943	1968	rBV	506468	865316	70.60%	9.499%
44	7.643	2028	2038	2065	rBV	99280	173129	14.13%	1.901%
45	7.836	2096	2098	2101	rBV2	252	132	0.01%	0.001%
46	7.939	2128	2130	2131	rBV2	273	71	0.01%	0.001%
47	8.000	2140	2149	2165	rVB3	8455	14663	1.20%	0.161%
48	8.068	2168	2170	2172	rBV	228	118	0.01%	0.001%
49	8.109	2172	2183	2220	rBV2	266039	556802	45.43%	6.112%
50	8.531	2312	2314	2317	rBV	345	190	0.02%	0.002%
51	8.672	2355	2358	2361	rBV2	503	332	0.03%	0.004%
52	8.733	2375	2377	2379	rVB2	421	171	0.01%	0.002%
53	8.791	2387	2395	2398	rBV3	590	688	0.06%	0.008%
54	8.807	2398	2400	2404	rBV2	352	268	0.02%	0.003%
55	8.871	2409	2420	2446	rBV	562960	910661	74.30%	9.997%
56	9.064	2479	2480	2482	rBV	209	102	0.01%	0.001%
57	9.231	2530	2532	2535	rVB	444	204	0.02%	0.002%
58	9.251	2535	2538	2541	rBV2	244	189	0.02%	0.002%
59	9.341	2564	2566	2569	rVB2	350	156	0.01%	0.002%
60	9.354	2569	2570	2571	rBV2	91	19	0.00%	0.000%
61	9.363	2571	2573	2575	rBV2	169	86	0.01%	0.001%
62	9.421	2587	2591	2596	rBV2	270	374	0.03%	0.004%
63	9.640	2656	2659	2661	rBV	241	169	0.01%	0.002%
64	9.678	2669	2671	2674	rVB2	298	120	0.01%	0.001%
65	9.801	2704	2709	2711	rBV2	347	303	0.02%	0.003%
66	9.897	2737	2739	2743	rBV	262	178	0.01%	0.002%
67	10.029	2777	2780	2784	rBV2	446	358	0.03%	0.004%
68	10.125	2806	2810	2813	rBV2	296	260	0.02%	0.003%
69	10.238	2833	2845	2861	rBV	276393	438296	35.76%	4.811%
70	10.341	2875	2877	2881	rBV2	361	287	0.02%	0.003%
71	10.518	2927	2932	2935	rBV2	294	290	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101920\
 Data File : VV018988.D
 Acq On : 20 Oct 2020 00:45
 Operator : SY/MD
 Sample : L4430-01 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

72	10.804	3018	3021	3022	rBV	232	147	0.01%	0.002%
73	10.842	3029	3033	3038	rBV2	262	301	0.02%	0.003%
74	10.878	3040	3044	3046	rVV2	270	215	0.02%	0.002%
75	10.913	3050	3055	3056	rBV	284	239	0.02%	0.003%
76	10.961	3067	3070	3074	rBV	456	292	0.02%	0.003%
77	11.270	3155	3166	3189	rBV	548634	841492	68.66%	9.238%
78	11.489	3232	3234	3236	rBV	338	173	0.01%	0.002%
79	11.646	3270	3283	3302	rBV	545138	844751	68.93%	9.273%
80	11.833	3338	3341	3343	rBV	393	243	0.02%	0.003%
81	12.341	3497	3499	3501	rBV2	394	215	0.02%	0.002%
82	12.524	3552	3556	3558	rBV	429	361	0.03%	0.004%
83	12.923	3675	3680	3682	rBV2	339	378	0.03%	0.004%
84	14.087	4040	4042	4047	rVB3	460	354	0.03%	0.004%


Sum of corrected areas: 9109409

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV101920\
Data File : VV018988.D
Acq On : 20 Oct 2020 00:45
Operator : SY/MD
Sample : L4430-01 40X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

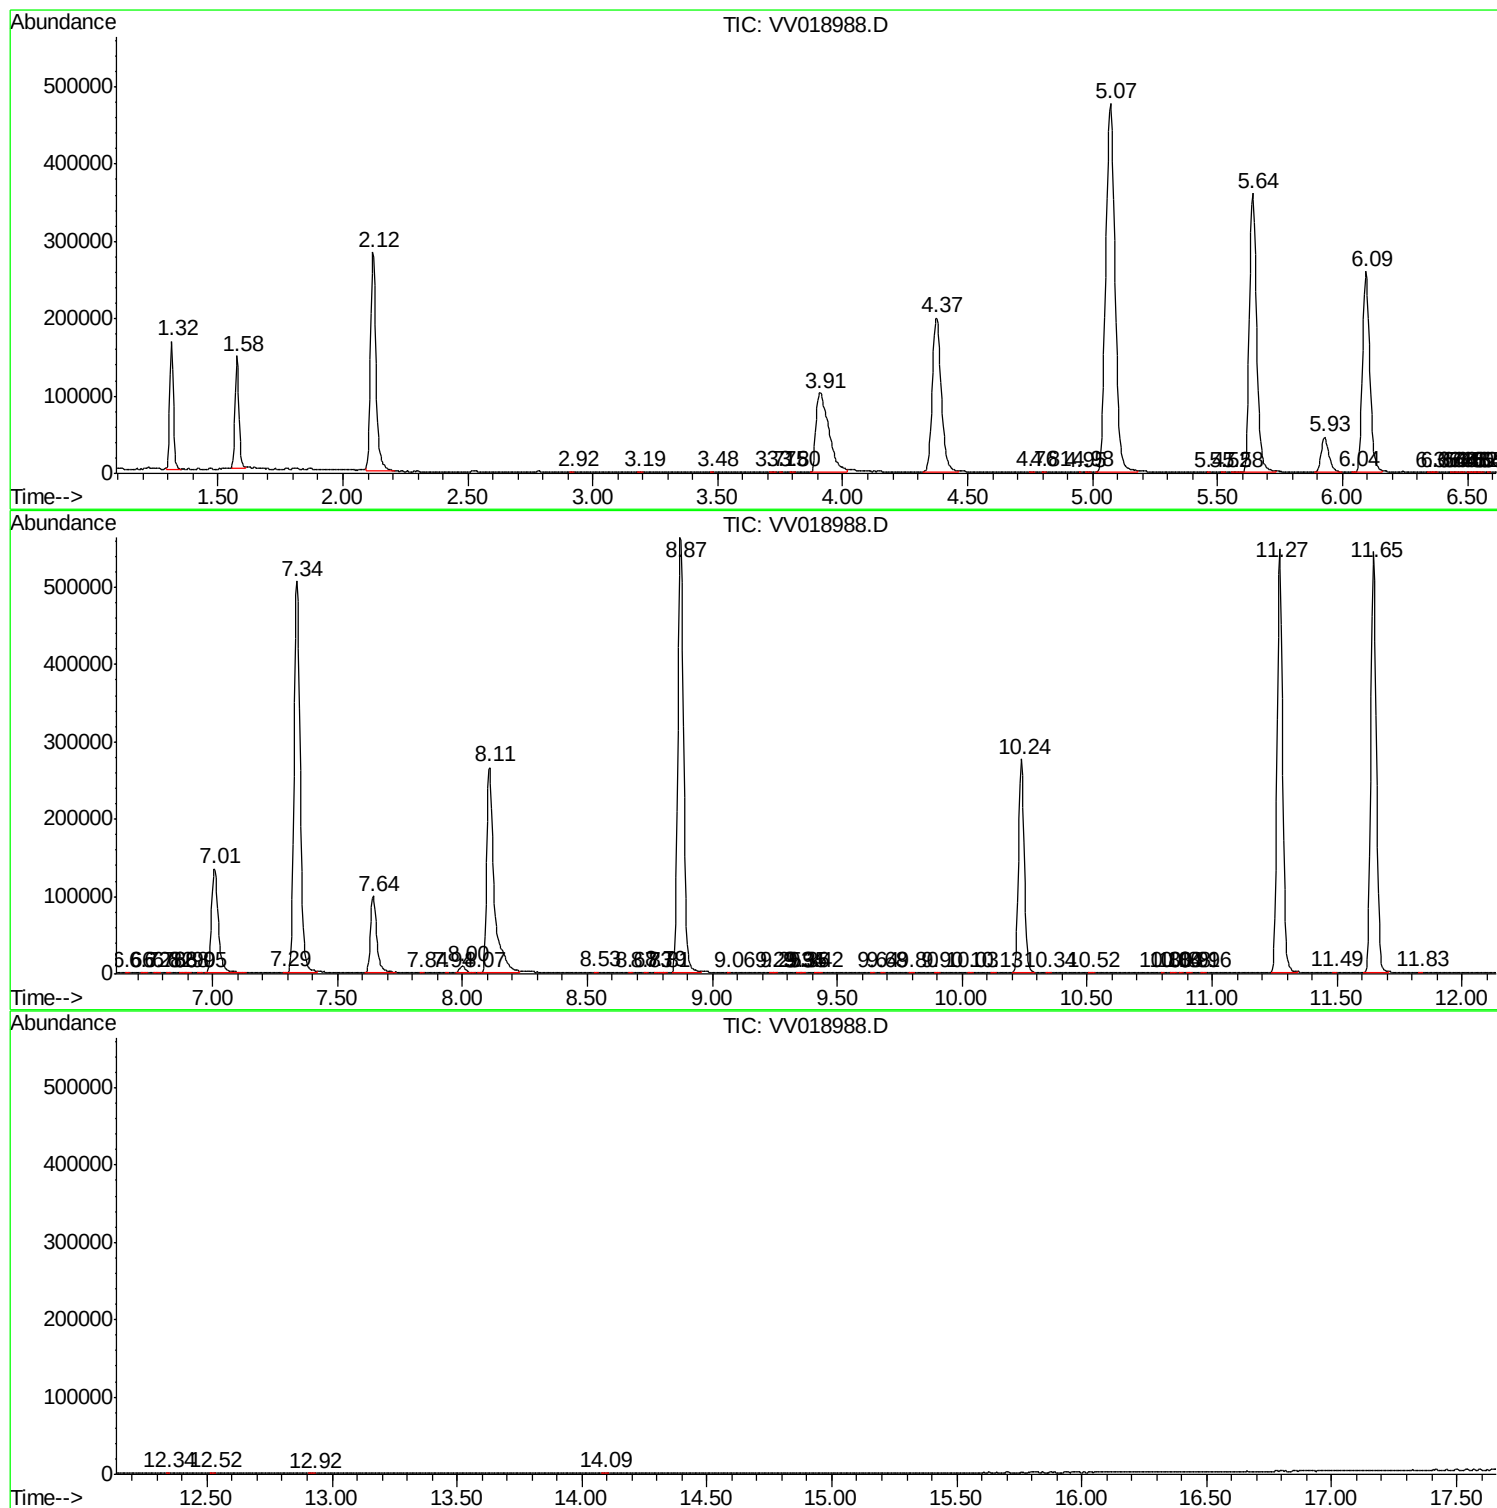

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV101920\
Data File : VV018988.D
Acq On : 20 Oct 2020 00:45
Operator : SY/MD
Sample : L4430-01 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV101920\
Data File : VV018988.D
Acq On : 20 Oct 2020 00:45
Operator : SY/MD
Sample : L4430-01 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc