

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101920\
 Data File : VV018989.D
 Acq On : 20 Oct 2020 01:09
 Operator : SY/MD
 Sample : L4430-02 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	82	rVB2	178748	186582	15.82%	2.025%
2	1.576	144	151	163	rVB	147623	162444	13.78%	1.763%
3	2.119	311	320	340	rVB	281353	432733	36.70%	4.696%
4	2.589	464	466	469	rBV	395	205	0.02%	0.002%
5	2.627	475	478	479	rBV2	773	473	0.04%	0.005%
6	2.781	516	526	538	rBV3	7621	14338	1.22%	0.156%
7	3.158	641	643	644	rVB3	292	66	0.01%	0.001%
8	3.248	667	671	675	rBV2	395	385	0.03%	0.004%
9	3.666	798	801	809	rVB3	686	622	0.05%	0.007%
10	3.907	865	876	909	rBV2	103986	363332	30.81%	3.943%
11	4.373	1005	1021	1049	rBV	197313	493213	41.83%	5.353%
12	5.003	1213	1217	1220	rBV3	417	367	0.03%	0.004%
13	5.071	1221	1238	1264	rBV2	456559	1179193	100.00%	12.797%
14	5.296	1306	1308	1312	rBV3	443	265	0.02%	0.003%
15	5.392	1336	1338	1340	rBV2	285	82	0.01%	0.001%
16	5.437	1349	1352	1355	rVB3	432	285	0.02%	0.003%
17	5.453	1355	1357	1360	rBV3	169	96	0.01%	0.001%
18	5.476	1360	1364	1367	rBV	372	293	0.02%	0.003%
19	5.640	1403	1415	1441	rBV	360395	725549	61.53%	7.874%
20	5.929	1494	1505	1531	rVB4	56965	134184	11.38%	1.456%
21	6.093	1542	1556	1580	rBV	263070	537705	45.60%	5.836%
22	6.312	1621	1624	1628	rVB2	383	274	0.02%	0.003%
23	6.334	1629	1631	1632	rBV	382	117	0.01%	0.001%
24	6.347	1633	1635	1639	rVB2	338	165	0.01%	0.002%
25	6.386	1644	1647	1650	rVB	243	166	0.01%	0.002%
26	6.457	1665	1669	1672	rBV2	364	226	0.02%	0.002%
27	6.473	1672	1674	1679	rVV2	173	102	0.01%	0.001%
28	6.521	1688	1689	1692	rBV	190	98	0.01%	0.001%
29	6.572	1703	1705	1708	rVB2	387	158	0.01%	0.002%
30	6.585	1708	1709	1711	rBV	234	100	0.01%	0.001%
31	6.633	1720	1724	1728	rBV2	549	448	0.04%	0.005%
32	6.675	1732	1737	1739	rBV4	632	582	0.05%	0.006%
33	6.752	1756	1761	1764	rBV	462	479	0.04%	0.005%
34	6.820	1777	1782	1785	rBV	581	461	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101920\
 Data File : VV018989.D
 Acq On : 20 Oct 2020 01:09
 Operator : SY/MD
 Sample : L4430-02 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

35	6.894	1801	1805	1808	rBV	532	344	0.03%	0.004%
36	6.923	1808	1814	1819	rVB3	297	352	0.03%	0.004%
37	6.948	1819	1822	1824	rBV2	272	172	0.01%	0.002%
38	6.965	1824	1827	1830	rBV	312	178	0.02%	0.002%
39	7.006	1830	1840	1862	rBV2	132989	247919	21.02%	2.691%
40	7.338	1931	1943	1963	rBV	515130	885430	75.09%	9.609%
41	7.643	2027	2038	2059	rBV	99058	175013	14.84%	1.899%
42	7.865	2105	2107	2111	rVB2	701	418	0.04%	0.005%
43	7.891	2111	2115	2116	rBV2	192	161	0.01%	0.002%
44	7.920	2121	2124	2128	rBV3	398	300	0.03%	0.003%
45	8.000	2139	2149	2162	rVB4	16789	29288	2.48%	0.318%
46	8.074	2170	2172	2173	rBV4	360	166	0.01%	0.002%
47	8.109	2173	2183	2220	rVV2	270383	563309	47.77%	6.113%
48	8.379	2265	2267	2270	rBV4	506	320	0.03%	0.003%
49	8.595	2332	2334	2337	rBV2	327	230	0.02%	0.002%
50	8.640	2345	2348	2350	rBV2	358	230	0.02%	0.002%
51	8.675	2357	2359	2362	rVB2	216	87	0.01%	0.001%
52	8.714	2369	2371	2374	rVB3	450	201	0.02%	0.002%
53	8.733	2374	2377	2378	rBV	190	112	0.01%	0.001%
54	8.784	2390	2393	2398	rVB3	411	430	0.04%	0.005%
55	8.813	2398	2402	2404	rBV	458	335	0.03%	0.004%
56	8.871	2408	2420	2447	rBV	563217	925590	78.49%	10.045%
57	9.183	2515	2517	2520	rBV	525	336	0.03%	0.004%
58	9.202	2520	2523	2524	rBV2	206	119	0.01%	0.001%
59	9.241	2533	2535	2536	rBV2	246	104	0.01%	0.001%
60	9.328	2558	2562	2564	rBV	289	264	0.02%	0.003%
61	9.389	2576	2581	2584	rBV	393	404	0.03%	0.004%
62	9.518	2618	2621	2625	rBV2	325	229	0.02%	0.002%
63	9.743	2685	2691	2695	rBV2	586	615	0.05%	0.007%
64	10.006	2771	2773	2778	rBV2	255	206	0.02%	0.002%
65	10.032	2779	2781	2784	rVB2	402	149	0.01%	0.002%
66	10.103	2800	2803	2805	rBV2	333	203	0.02%	0.002%
67	10.157	2818	2820	2822	rBV	220	124	0.01%	0.001%
68	10.238	2832	2845	2862	rBV	279761	441564	37.45%	4.792%
69	10.334	2871	2875	2880	rBV3	319	274	0.02%	0.003%
70	10.427	2902	2904	2908	rVB2	451	270	0.02%	0.003%
71	10.447	2908	2910	2911	rBV2	221	99	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101920\
 Data File : VV018989.D
 Acq On : 20 Oct 2020 01:09
 Operator : SY/MD
 Sample : L4430-02 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

72	10.620	2958	2964	2967	rBV2	377	469	0.04%	0.005%
73	10.791	3012	3017	3022	rBV	481	514	0.04%	0.006%
74	10.919	3055	3057	3060	rBV	198	109	0.01%	0.001%
75	11.138	3121	3125	3130	rVB2	555	496	0.04%	0.005%
76	11.167	3130	3134	3141	rBV	403	440	0.04%	0.005%
77	11.199	3141	3144	3147	rBV	322	249	0.02%	0.003%
78	11.270	3155	3166	3185	rBV	559853	846382	71.78%	9.185%
79	11.646	3271	3283	3305	rBV	553527	853446	72.38%	9.262%
80	11.852	3345	3347	3350	rBV	423	216	0.02%	0.002%
81	12.251	3469	3471	3477	rVB2	302	213	0.02%	0.002%
82	12.566	3567	3569	3573	rBV2	313	201	0.02%	0.002%
83	13.135	3743	3746	3749	rBV2	453	293	0.02%	0.003%


Sum of corrected areas: 9214361

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV101920\
Data File : VV018989.D
Acq On : 20 Oct 2020 01:09
Operator : SY/MD
Sample : L4430-02 40X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

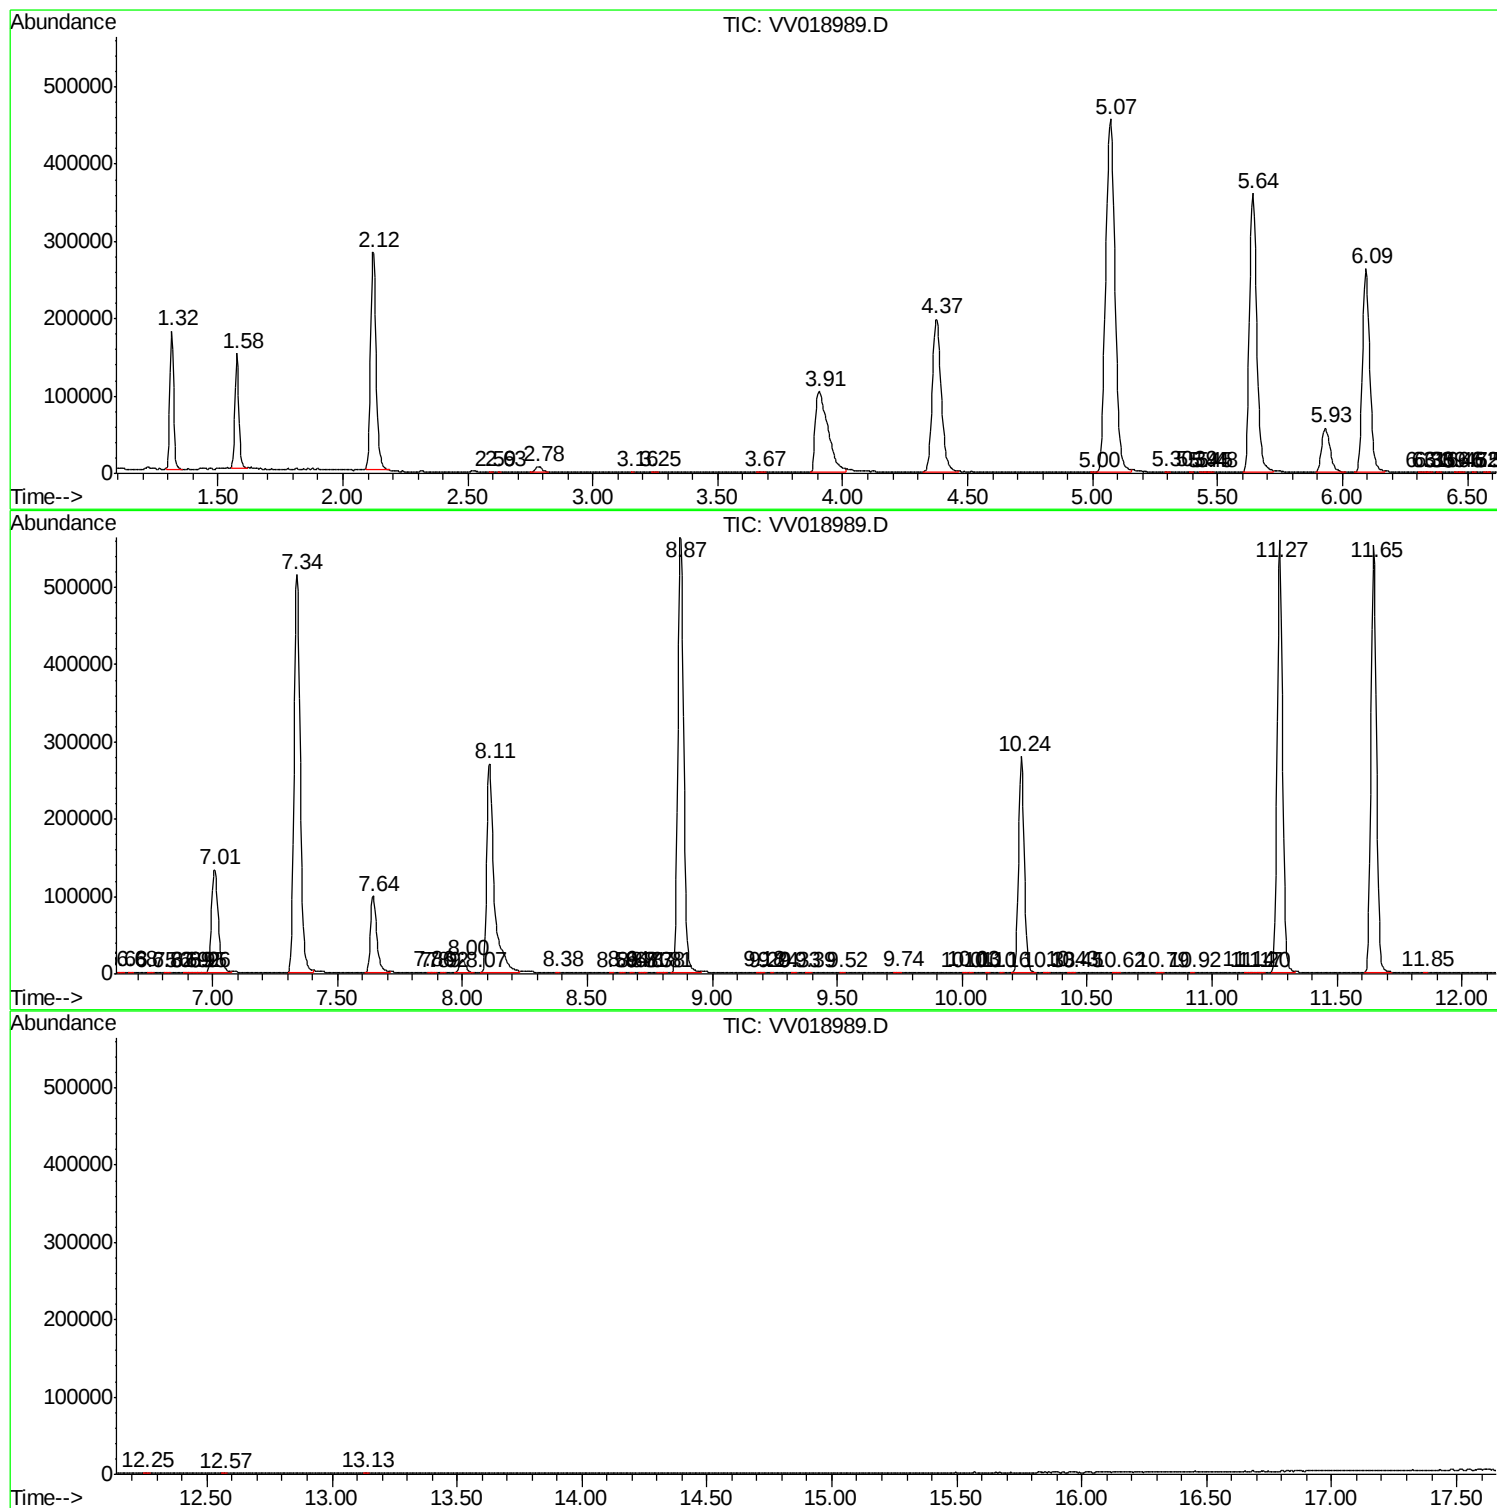

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV101920\
Data File : VV018989.D
Acq On : 20 Oct 2020 01:09
Operator : SY/MD
Sample : L4430-02 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV101920\
Data File : VV018989.D
Acq On : 20 Oct 2020 01:09
Operator : SY/MD
Sample : L4430-02 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc