

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101920\
 Data File : VV018991.D
 Acq On : 20 Oct 2020 01:56
 Operator : SY/MD
 Sample : L4430-05DL 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB4DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	82	rVB	158993	156178	13.46%	1.454%
2	1.576	144	151	167	rBV	148396	165106	14.23%	1.537%
3	2.119	311	320	348	rVB	279759	439021	37.84%	4.086%
4	2.663	487	489	493	rBV3	375	243	0.02%	0.002%
5	2.778	518	525	537	rBV6	3554	6705	0.58%	0.062%
6	2.871	548	554	559	rBV3	583	710	0.06%	0.007%
7	3.026	598	602	605	rBV2	404	301	0.03%	0.003%
8	3.328	692	696	699	rBV3	531	493	0.04%	0.005%
9	3.351	701	703	707	rVB	530	350	0.03%	0.003%
10	3.431	722	728	731	rBV2	442	472	0.04%	0.004%
11	3.492	746	747	750	rBV	282	187	0.02%	0.002%
12	3.707	812	814	816	rBV	388	155	0.01%	0.001%
13	3.933	866	884	915	rBV3	152049	560488	48.30%	5.216%
14	4.376	1006	1022	1051	rBV	196055	491032	42.32%	4.570%
15	4.862	1168	1173	1176	rBV3	542	528	0.05%	0.005%
16	4.916	1187	1190	1193	rVB	358	238	0.02%	0.002%
17	4.933	1193	1195	1198	rVB2	306	154	0.01%	0.001%
18	4.958	1198	1203	1206	rBV2	462	557	0.05%	0.005%
19	4.994	1211	1214	1217	rBV	463	324	0.03%	0.003%
20	5.071	1221	1238	1264	rBV2	450341	1160334	100.00%	10.799%
21	5.444	1352	1354	1356	rBV2	592	274	0.02%	0.003%
22	5.460	1356	1359	1365	rVB4	573	544	0.05%	0.005%
23	5.489	1365	1368	1369	rBV	298	184	0.02%	0.002%
24	5.582	1395	1397	1400	rVB	244	113	0.01%	0.001%
25	5.640	1403	1415	1443	rBV	362619	732415	63.12%	6.816%
26	5.936	1492	1507	1531	rBV3	142675	322788	27.82%	3.004%
27	6.093	1543	1556	1579	rBV	266474	538943	46.45%	5.016%
28	6.312	1621	1624	1627	rBV2	359	191	0.02%	0.002%
29	6.418	1655	1657	1662	rBV	106	81	0.01%	0.001%
30	6.473	1671	1674	1676	rVB	253	128	0.01%	0.001%
31	6.489	1676	1679	1680	rBV2	320	186	0.02%	0.002%
32	6.521	1687	1689	1691	rBV	189	69	0.01%	0.001%
33	6.553	1697	1699	1700	rBV	187	68	0.01%	0.001%
34	6.579	1705	1707	1711	rVB2	341	183	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101920\
 Data File : VV018991.D
 Acq On : 20 Oct 2020 01:56
 Operator : SY/MD
 Sample : L4430-05DL 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB4DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

35	6.604	1712	1715	1718	rBV2	296	189	0.02%	0.002%
36	6.627	1719	1722	1725	rVB	238	128	0.01%	0.001%
37	6.656	1730	1731	1733	rBV2	298	108	0.01%	0.001%
38	6.826	1782	1784	1788	rVB	461	201	0.02%	0.002%
39	6.852	1788	1792	1794	rBV2	318	223	0.02%	0.002%
40	6.900	1800	1807	1810	rBV2	353	383	0.03%	0.004%
41	6.916	1810	1812	1813	rBV2	255	112	0.01%	0.001%
42	7.006	1829	1840	1863	rBV	134881	248963	21.46%	2.317%
43	7.338	1930	1943	1965	rBV	514382	882940	76.09%	8.217%
44	7.572	2013	2016	2020	rVB4	680	564	0.05%	0.005%
45	7.592	2020	2022	2023	rBV4	242	120	0.01%	0.001%
46	7.643	2028	2038	2061	rBV	99226	175405	15.12%	1.632%
47	7.939	2126	2130	2135	rBV2	379	357	0.03%	0.003%
48	7.997	2135	2148	2173	rBV	697521	1153332	99.40%	10.734%
49	8.109	2173	2183	2219	rBV2	277505	567864	48.94%	5.285%
50	8.479	2296	2298	2301	rVB2	510	224	0.02%	0.002%
51	8.518	2305	2310	2314	rBV3	409	470	0.04%	0.004%
52	8.662	2352	2355	2357	rBV	253	127	0.01%	0.001%
53	8.784	2391	2393	2396	rBV2	294	209	0.02%	0.002%
54	8.871	2409	2420	2447	rBV	583079	937505	80.80%	8.725%
55	9.145	2503	2505	2509	rBV3	266	236	0.02%	0.002%
56	9.202	2521	2523	2526	rBV3	372	287	0.02%	0.003%
57	9.289	2548	2550	2553	rBV	287	86	0.01%	0.001%
58	9.347	2566	2568	2573	rVB2	349	233	0.02%	0.002%
59	9.498	2613	2615	2616	rBV	266	105	0.01%	0.001%
60	9.601	2645	2647	2649	rBV	167	101	0.01%	0.001%
61	9.698	2674	2677	2678	rBV	188	108	0.01%	0.001%
62	9.755	2693	2695	2696	rBV	338	115	0.01%	0.001%
63	9.916	2741	2745	2749	rBV	350	272	0.02%	0.003%
64	9.948	2753	2755	2758	rBV2	308	185	0.02%	0.002%
65	10.022	2774	2778	2780	rBV	673	481	0.04%	0.004%
66	10.093	2794	2800	2803	rBV	502	435	0.04%	0.004%
67	10.238	2832	2845	2864	rBV	289429	450607	38.83%	4.194%
68	10.350	2878	2880	2881	rBV	290	114	0.01%	0.001%
69	10.431	2903	2905	2907	rBV	289	151	0.01%	0.001%
70	10.456	2911	2913	2914	rBV	220	67	0.01%	0.001%
71	10.537	2936	2938	2941	rBV2	303	152	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101920\
 Data File : VV018991.D
 Acq On : 20 Oct 2020 01:56
 Operator : SY/MD
 Sample : L4430-05DL 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB4DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

72	10.685	2982	2984	2987	rBV2	226	168	0.01%	0.002%
73	10.714	2990	2993	2998	rVV2	390	279	0.02%	0.003%
74	10.813	3021	3024	3029	rBV3	340	288	0.02%	0.003%
75	10.952	3064	3067	3071	rBV2	394	291	0.03%	0.003%
76	10.974	3071	3074	3075	rBV2	420	227	0.02%	0.002%
77	11.067	3101	3103	3107	rBV	256	205	0.02%	0.002%
78	11.106	3113	3115	3122	rVB2	328	239	0.02%	0.002%
79	11.218	3147	3150	3151	rBV	396	221	0.02%	0.002%
80	11.270	3154	3166	3187	rBV	562556	869239	74.91%	8.090%
81	11.492	3231	3235	3239	rBV3	572	511	0.04%	0.005%
82	11.646	3271	3283	3302	rBV	558549	867918	74.80%	8.078%
83	11.871	3349	3353	3357	rVB3	372	315	0.03%	0.003%
84	11.961	3378	3381	3383	rBV2	396	301	0.03%	0.003%
85	12.077	3415	3417	3418	rBV	302	119	0.01%	0.001%
86	12.099	3422	3424	3427	rBV	253	145	0.01%	0.001%
87	12.379	3506	3511	3516	rBV3	470	584	0.05%	0.005%
88	12.649	3593	3595	3599	rBV2	352	275	0.02%	0.003%
89	12.871	3662	3664	3666	rBV2	367	169	0.01%	0.002%
90	13.103	3734	3736	3737	rBV2	348	106	0.01%	0.001%
91	13.283	3789	3792	3793	rBV	401	234	0.02%	0.002%
92	13.765	3941	3942	3943	rBV	390	121	0.01%	0.001%


Sum of corrected areas: 10744857

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV101920\
Data File : VV018991.D
Acq On : 20 Oct 2020 01:56
Operator : SY/MD
Sample : L4430-05DL 40X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB4DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

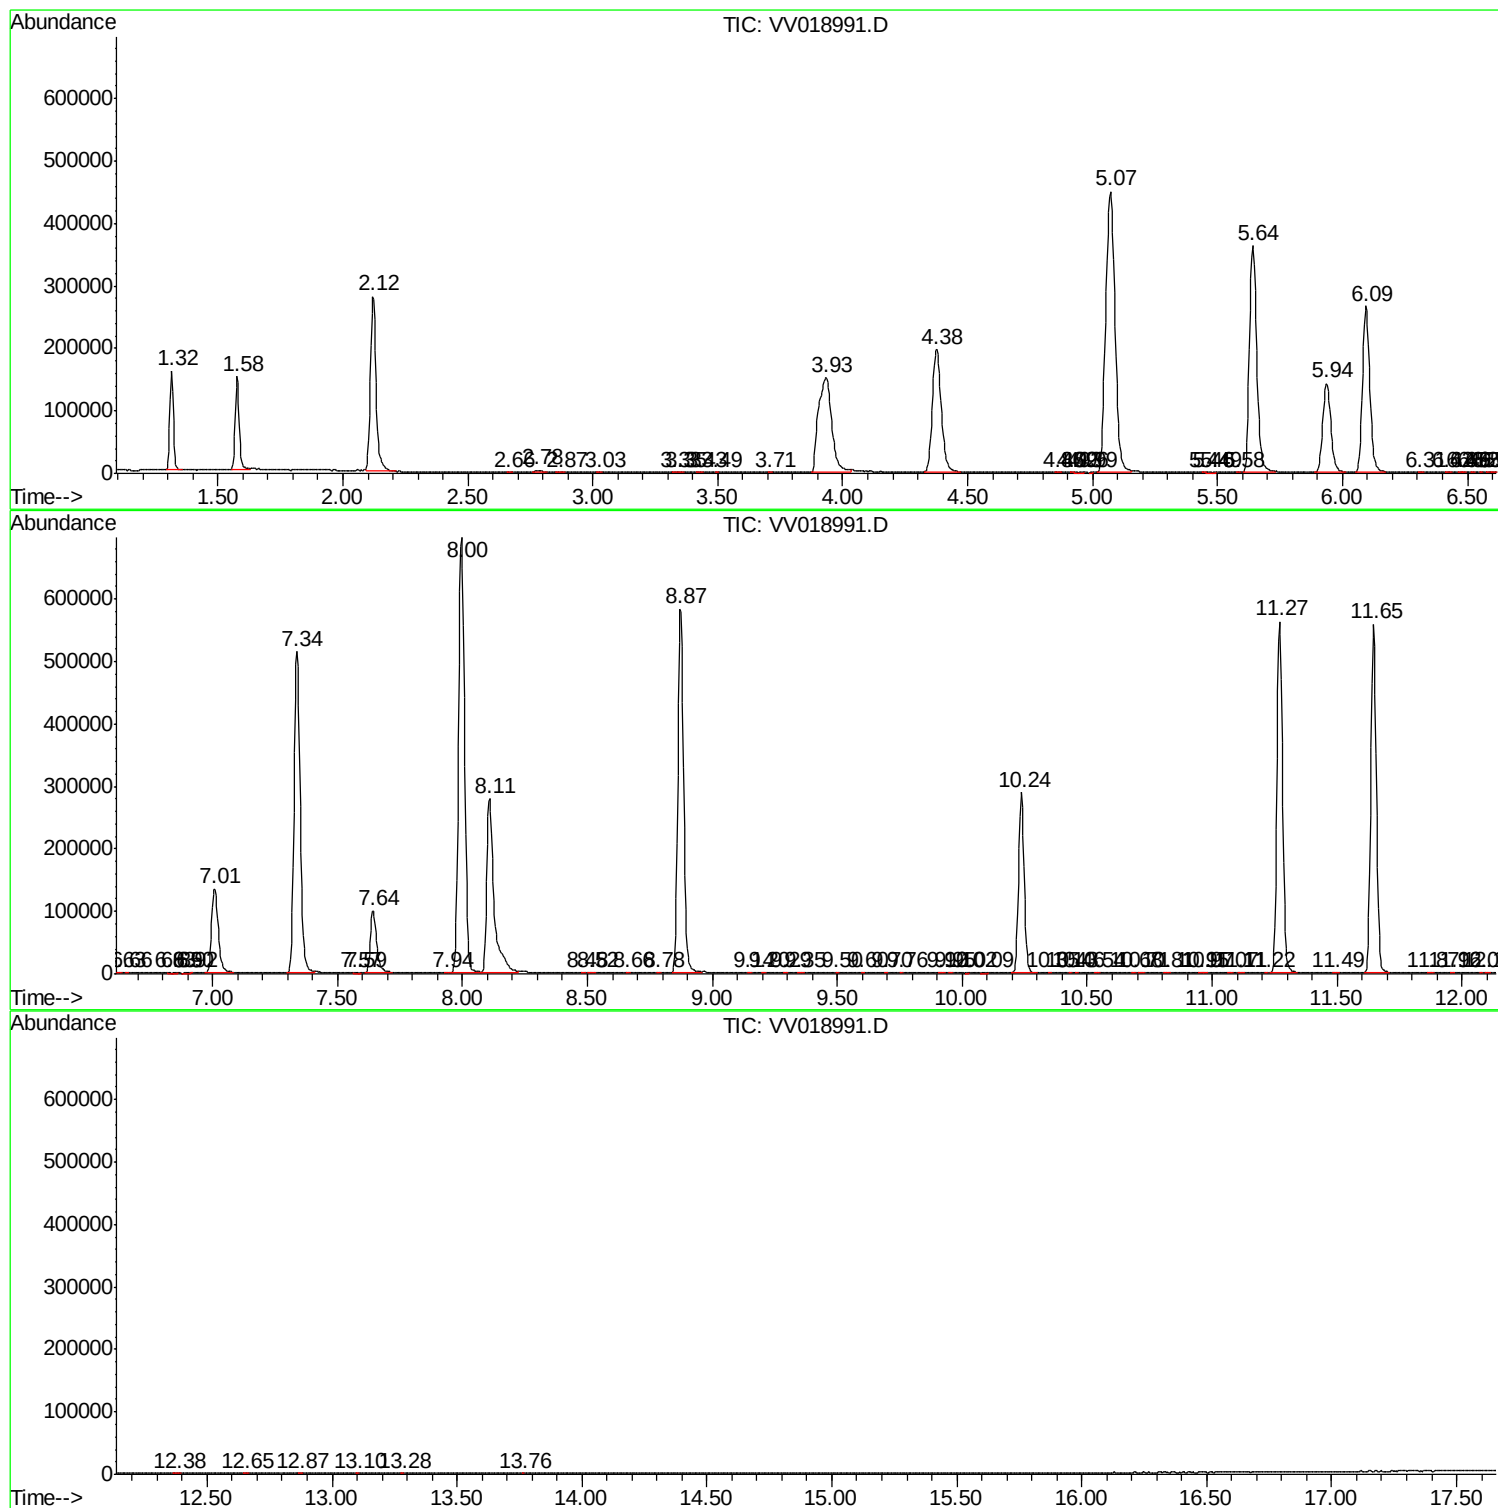

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV101920\
Data File : VV018991.D
Acq On : 20 Oct 2020 01:56
Operator : SY/MD
Sample : L4430-05DL 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB4DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV101920\
Data File : VV018991.D
Acq On : 20 Oct 2020 01:56
Operator : SY/MD
Sample : L4430-05DL 40X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0AB4DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc