

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101920\
 Data File : VV018992.D
 Acq On : 20 Oct 2020 02:20
 Operator : SY/MD
 Sample : L4430-06DL 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	81	rVB	146435	149650	12.07%	1.430%
2	1.576	144	151	165	rVB	145817	160698	12.96%	1.535%
3	2.119	311	320	347	rVB	263233	414232	33.41%	3.957%
4	2.785	518	527	537	rBV4	5151	8383	0.68%	0.080%
5	3.206	653	658	659	rBV2	440	398	0.03%	0.004%
6	3.347	699	702	704	rBV2	349	226	0.02%	0.002%
7	3.859	858	861	865	rBV2	360	328	0.03%	0.003%
8	3.933	865	884	924	rBV2	155937	584707	47.16%	5.586%
9	4.283	989	993	996	rBV2	399	359	0.03%	0.003%
10	4.373	1005	1021	1056	rBV	176650	446731	36.03%	4.268%
11	4.598	1085	1091	1094	rBV	569	516	0.04%	0.005%
12	4.640	1101	1104	1106	rBV	349	160	0.01%	0.002%
13	4.653	1106	1108	1109	rBV	421	191	0.02%	0.002%
14	4.746	1134	1137	1139	rBV2	369	286	0.02%	0.003%
15	4.769	1142	1144	1145	rBV	229	110	0.01%	0.001%
16	4.826	1159	1162	1165	rBV	287	175	0.01%	0.002%
17	4.859	1168	1172	1173	rBV	279	193	0.02%	0.002%
18	4.884	1178	1180	1183	rVB	353	159	0.01%	0.002%
19	4.945	1196	1199	1205	rVB3	341	308	0.02%	0.003%
20	4.974	1205	1208	1212	rVB3	284	185	0.01%	0.002%
21	5.003	1212	1217	1219	rBV	257	236	0.02%	0.002%
22	5.013	1219	1220	1221	rVB	255	49	0.00%	0.000%
23	5.071	1221	1238	1260	rBV2	438380	1092721	88.14%	10.439%
24	5.431	1347	1350	1355	rVB3	531	435	0.04%	0.004%
25	5.486	1363	1367	1371	rBV3	350	396	0.03%	0.004%
26	5.553	1386	1388	1392	rVB2	322	169	0.01%	0.002%
27	5.640	1403	1415	1444	rBV	342185	684359	55.20%	6.538%
28	5.936	1493	1507	1536	rBV3	168350	381102	30.74%	3.641%
29	6.093	1543	1556	1583	rBV	287795	582191	46.96%	5.562%
30	6.447	1664	1666	1669	rBV2	501	306	0.02%	0.003%
31	6.482	1676	1677	1679	rBV	281	113	0.01%	0.001%
32	6.579	1704	1707	1712	rVB3	467	421	0.03%	0.004%
33	6.608	1712	1716	1719	rBV3	621	502	0.04%	0.005%
34	6.791	1771	1773	1777	rVB	251	108	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101920\
 Data File : VV018992.D
 Acq On : 20 Oct 2020 02:20
 Operator : SY/MD
 Sample : L4430-06DL 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

35	6.814	1777	1780	1783	rBV2	408	255	0.02%	0.002%
36	6.916	1810	1812	1816	rBV2	166	110	0.01%	0.001%
37	6.936	1816	1818	1821	rVB2	265	132	0.01%	0.001%
38	6.968	1821	1828	1830	rBV3	343	453	0.04%	0.004%
39	7.010	1830	1841	1864	rBV	130708	242170	19.53%	2.314%
40	7.215	1903	1905	1908	rBV4	427	255	0.02%	0.002%
41	7.338	1930	1943	1966	rBV	476951	821528	66.26%	7.849%
42	7.643	2027	2038	2060	rBV	96186	171514	13.83%	1.639%
43	7.849	2100	2102	2105	rBV2	314	179	0.01%	0.002%
44	7.904	2115	2119	2121	rVB	517	396	0.03%	0.004%
45	7.923	2121	2125	2129	rBV3	255	245	0.02%	0.002%
46	7.997	2135	2148	2167	rBV	744123	1239797	100.00%	11.845%
47	8.109	2173	2183	2219	rBV3	266637	556050	44.85%	5.312%
48	8.466	2291	2294	2295	rBV3	510	295	0.02%	0.003%
49	8.653	2350	2352	2354	rBV2	520	252	0.02%	0.002%
50	8.688	2360	2363	2365	rBV2	172	113	0.01%	0.001%
51	8.698	2365	2366	2370	rVV	271	154	0.01%	0.001%
52	8.810	2398	2401	2404	rBV	247	172	0.01%	0.002%
53	8.833	2406	2408	2409	rBV	323	108	0.01%	0.001%
54	8.871	2409	2420	2445	rBV	547615	886510	71.50%	8.469%
55	9.080	2480	2485	2486	rBV4	468	447	0.04%	0.004%
56	9.180	2512	2516	2520	rVB	389	354	0.03%	0.003%
57	9.212	2524	2526	2533	rVB2	420	388	0.03%	0.004%
58	9.321	2554	2560	2565	rBV2	381	615	0.05%	0.006%
59	9.556	2630	2633	2634	rBV	298	144	0.01%	0.001%
60	9.637	2654	2658	2659	rBV2	365	255	0.02%	0.002%
61	9.752	2693	2694	2695	rBV2	78	30	0.00%	0.000%
62	9.945	2751	2754	2757	rBV	281	202	0.02%	0.002%
63	10.013	2771	2775	2776	rBV2	320	201	0.02%	0.002%
64	10.077	2792	2795	2800	rVB3	452	418	0.03%	0.004%
65	10.238	2834	2845	2865	rBV	273963	438063	35.33%	4.185%
66	10.347	2874	2879	2884	rBV2	512	580	0.05%	0.006%
67	10.399	2892	2895	2896	rBV	301	138	0.01%	0.001%
68	10.543	2936	2940	2942	rBV2	330	201	0.02%	0.002%
69	10.592	2949	2955	2956	rBV2	408	385	0.03%	0.004%
70	10.665	2975	2978	2980	rBV2	231	140	0.01%	0.001%
71	10.694	2985	2987	2989	rBV	348	212	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101920\
Data File : VV018992.D
Acq On : 20 Oct 2020 02:20
Operator : SY/MD
Sample : L4430-06DL 40X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB5DL

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Title : VOC Analysis

72	10.852	3033	3036	3040	rBV3	196	156	0.01%	0.001%
73	10.926	3055	3059	3062	rBV2	330	219	0.02%	0.002%
74	10.945	3062	3065	3067	rBV	263	176	0.01%	0.002%
75	11.071	3102	3104	3105	rBV	151	48	0.00%	0.000%
76	11.270	3154	3166	3189	rBV	514657	794503	64.08%	7.590%
77	11.646	3271	3283	3307	rBV	511958	796146	64.22%	7.606%
78	12.251	3467	3471	3474	rBV2	419	330	0.03%	0.003%
79	12.270	3475	3477	3479	rBV2	322	155	0.01%	0.001%
80	12.826	3647	3650	3651	rBV	380	208	0.02%	0.002%
81	13.646	3903	3905	3910	rBV	397	309	0.02%	0.003%
82	13.900	3980	3984	3985	rBV	541	368	0.03%	0.004%


Sum of corrected areas: 10467182

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV101920\
Data File : VV018992.D
Acq On : 20 Oct 2020 02:20
Operator : SY/MD
Sample : L4430-06DL 40X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

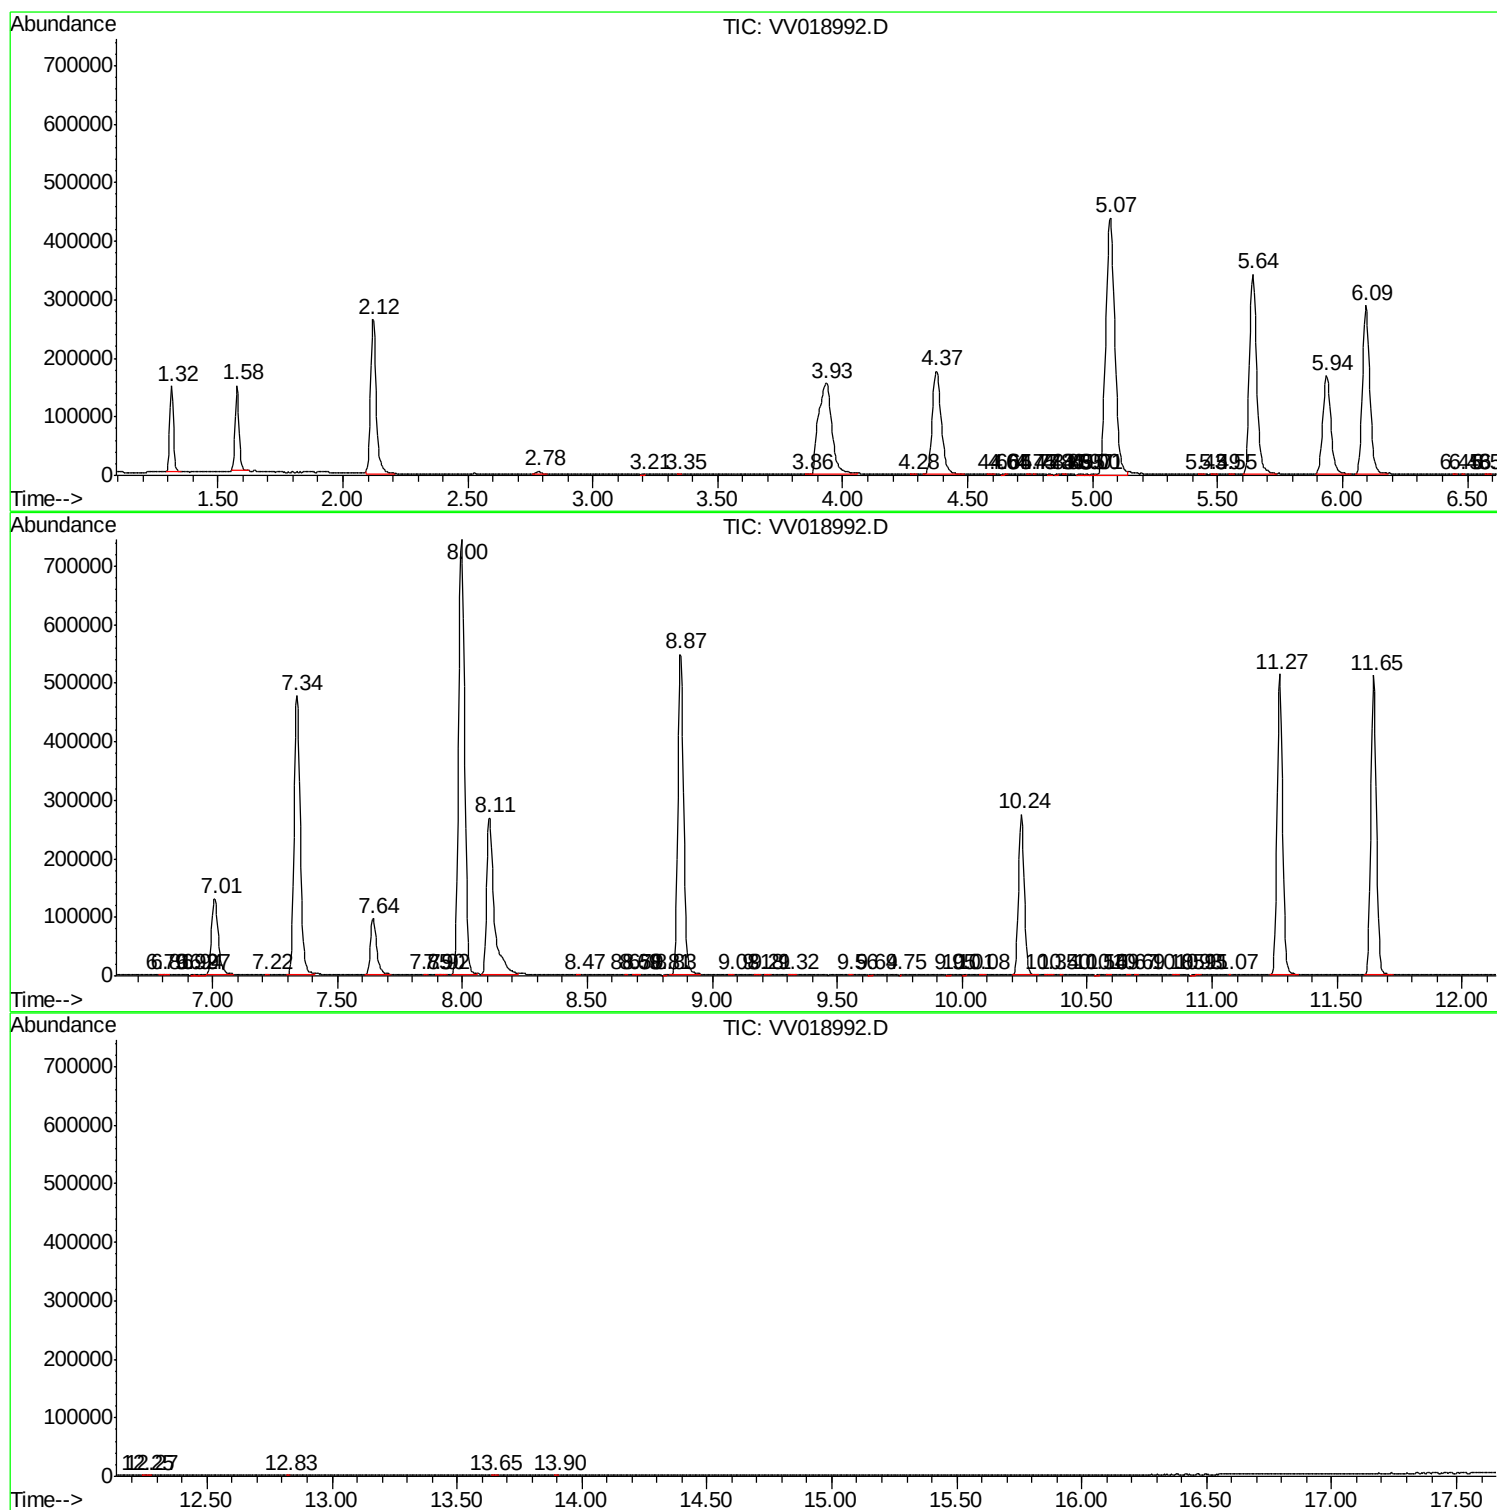

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV101920\
Data File : VV018992.D
Acq On : 20 Oct 2020 02:20
Operator : SY/MD
Sample : L4430-06DL 40X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0AB5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV101920\
Data File : VV018992.D
Acq On : 20 Oct 2020 02:20
Operator : SY/MD
Sample : L4430-06DL 40X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0AB5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc